NOTES CONTINUED: (5) SCRIBE, ENGRAVE, OR MECHANICALLY STAMP (NO INKS OR DYES) DRAWING PART NUMBER AND REVISION ON NOTED SURFACE FOLLOWED ON THE **NEXT LINE BY A THREE DIGIT SERIAL NUMBER. SERIAL** NUMBERS START AT 001 FOR THE FIRST ARTICLE AND PROCEED CONSECUTIVELY. USE .07" HIGH CHARACTERS. **EXAMPLE**: DXXXXXXX-VY, S/N 001.

VIBRATORY TOOL MAY BE USED. 6. APPROXIMATE WEIGHT = X.XXX LB.

7. MACHINE ALL SURFACES TO REMOVE OXIDES AND MILL FINISH, USE OF ABRASIVE REMOVAL TECHNIQUES IS NOT ALLOWED. REFER TO LIGO-E0900364

8. ALL PARTS SHALL BE MANUFACTURED IN ACCORDANCE WITH LIGO SPECIFICATION E0900364.

9. ALL HELI-COIL HOLES TO BE PREPARED ACCORDING TO EMHART HELI-COIL PRODUCT CATALOG, HC2000, REV 4

10. ALL HELI-COIL INSERTS TO BE INSTALLED BY LIGO PERSONNEL, AFTER DELIVERY OF FINISHED PARTS, USE NITRONIC 60 THREADED INSERTS.

11. ALL MATERIAL IS TO BE VIRGIN MATERIAL (i.e. NO WELD REPAIRS, PLUGS OR RECYCLED MATERIAL). NO REPÀIRS SHALL BE MADE UNLESS APPROVED IN ADVANCE, AND IN WRITING, BY LIGO LABORATORY.

12. SURFACE FINISH TO BE AS-PROCESSED FROM MILL/SUPPLIER, FREE FROM SCRATCHES OR GOUGES.


13. PART WILL BE PORCELAIN COATED PER LIGO SPECIFICATION E1000083 AFTER FABRICATION. THE INDICATED HOLES WILL BE MASKED PRIOR TO PORCELAIN COATING TO APPROXIMATELY 2.5-3X HOLE DIAMETER

14. DIMENSIONS APPLY BEFORE PORCELAIN COATING UNLESS SPECIFIED.

CENTERED ON BOTH SIDES OF THE HOLE.

15. BEND RADIUS: UNLESS OTHERWISE NOTED, THE BEND RADIUS SHOULD BE THE MINIMUM REQUIRED TO FORM WITHOUT CRACKING OR REQUIRING ADDITIONAL WORK WHEN FORMING. IN PARTICULAR IF SHEET METAL IS TO BE PORCELAIN COATED, THE BEND RADIUS SHALL BE A MINIMUM OF .12" OUTSIDE RADIUS OF BEND UNLESS

NOTES 13 and 14 DO NOT APPLY TO THIS PART

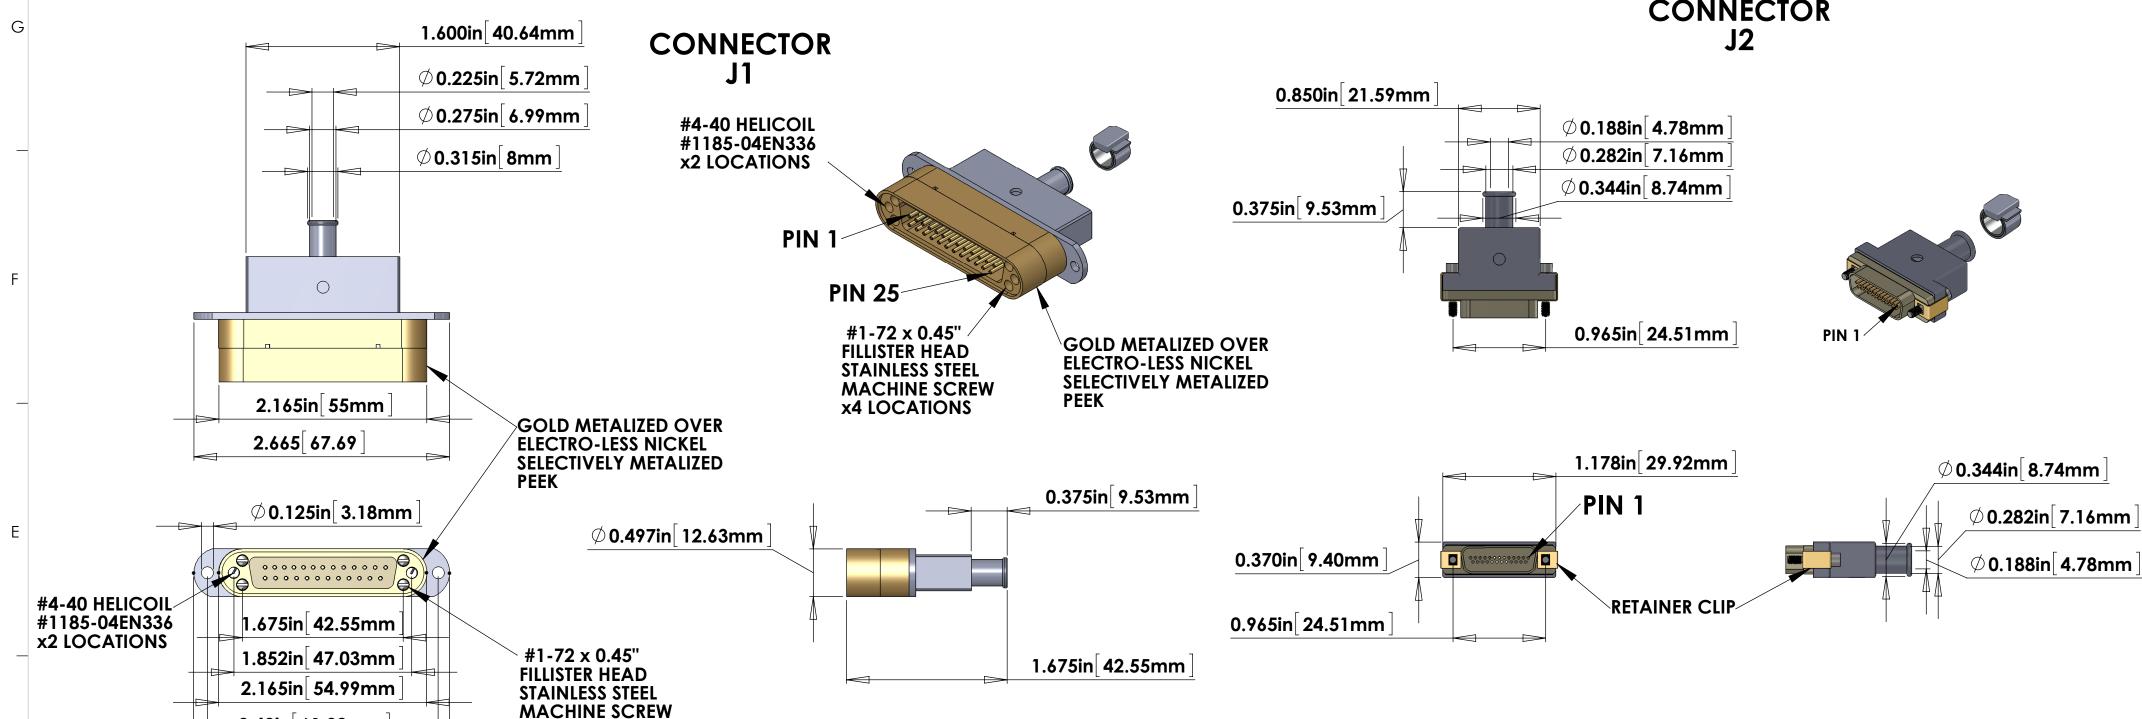

ITEM NO.	PART NUMBER	DESCRIPTION	QTY.	LENGTH
1	TICOR PART # TS0086-1 (TS0149-25CG20BS1-225F)	DB25 MALE CONNECTOR (J1) FOR UHV (GOLD METALIZED PEEK)		
2		DB25 CONNECTOR BACKSHELL FOR UHV (STAINLESS)	ı	
3	Glenair # DCDM255-5-MC216-225-240	MicroD25 FEMALE CONNECTOR (J2) FOR UHV	1	
4	Glenair # 500T010M25H06	MicroD25 CONNECTOR BACKSHELL FOR UHV	1	
5	C1	25 COND. (12 TW PAIR + 1 WIRE + SHIELD) CABLE WITH COPPER BRAID (SHIELD) 6 AND PEEK OVERBRAID 7		
6	CONTINENTAL PART #24x4x40BC	COPPER BRAID - CONTINENTAL CORDAGE PART #24x4x40BC	1	53in *
7	PART #6759	PEEK BRAID - PART #6759 MANUFACTURED WITH ZEUS 0.016" BLACK PEEK DRAWN MONOFILAMENT		
8	GLENAIR # 600-052 or BAND-IT # A10086	GLENAIR # 600-052 STANDARD BRAID CLAMP or BAND-IT PART # A10086 (0.240" WIDE) ("BAG OF 100" # A10089)	2	

x4 LOCATIONS

* NOTE: THE OVERALL LENGTH IS MEASURED FROM PIN TIP (25 PIN D-SUB) TO PIN TIP (25 PIN µD) OF THE CABLE. USE WHATEVER LENGTH IS NECESSARY FOR THE INTERNAL WIRING OF THE CONNECTORS AND STRIP LENGTH TO ACHIEVE THE CORRECT OVERALL LENGTH.

NOTES: (UNLESS OTHERWISE SPECIFIED)

2.40in 61.02mm

2.665in 67.69mm

MATERIAL: a. CONNECTOR SHELL - J1 - GOLD OVER ELECTRO-LESS NICKEL SELECTIVELY METALIZED PEEK VICTREX 450GL30.

b. CONNECTOR SHELL - J2 - PEEK VICTREX 450GL30.

c. BACKSHELL - STAINLESS STEEL WITH VENT HOLE. d. CONTACTS - BERYLLIUM COPPER ALLOY C17300

0.000050 MIN. GOLD OVER NICKEL.


e. HARDWARE: STAINLESS STEEL, PASSIVATED.


f. PEEK BRAID - PEEK VICTREX GRADE TDS-450CA30 CARBON LOADED - SUPPLIED BY LIGO.

B. CABLE 25 COND. 28 AWG, (40 STRD 44 AWG) WITH 2 LAYERS OF KAPTON TAPE. 12 TWISTED PAIRS (4 TO 5 TWISTS PER INCH) + 1 WIRE. OVERALL 40AWG COPPER BRAID 90% COVERAGE. OVERALL PEEK BRAID MIN. 50% COVERAGE. OVERALL CABLE O.D. WILL BE 0.240 IN.

C. CONNECTORS WILL BE SUPPLIED WITH HARDWARE. SCREWS SHOULD BE THE PROPER LENGTH FOR MATING.

CONNECTOR

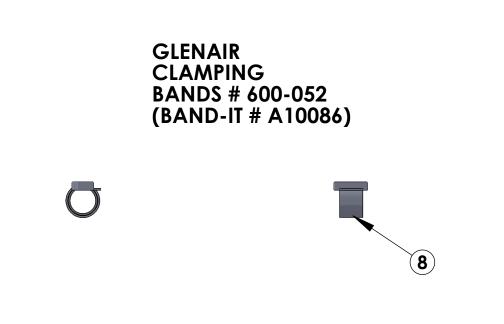

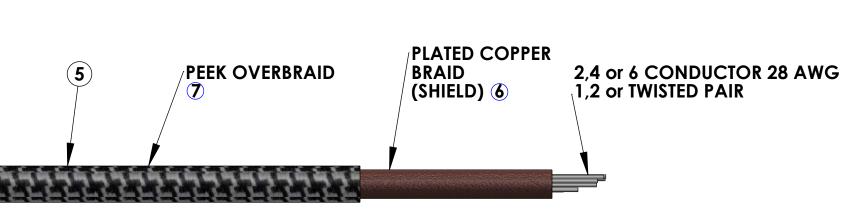

2. REMOVE ALL SHARP EDGES, .005-.015. FOR MACHINED PARTS. ROUND

NOTES AND TOLERANCES: (UNLESS OTHERWISE SPECIFIED)

3. DO NOT SCALE FROM DRAWING.

DIMENSIONS ARE IN

TOLERANCES:

ANGULAR ±

.XX ±

.XXX ±

. INTERPRET DRAWING PER ASME Y14.5-1994.

ALL EDGES APPROXIMATLEY R.02 FOR SHEET METAL PARTS.

SOLUBLE AND FREE OF SULFUR, SILICONE, AND CHLORINE.

4. ALL MACHINING FLUIDS MUST BE FULLY SYNTHETIC, FULLY WATER

SYSTEM

LIGO

NEXT ASSY

μınch

SUS

CALIFORNIA INSTITUTE OF TECHNOLOGY LIGO MASSACHUSETTS INSTITUTE OF TECHNOLOGY SUB-SYSTEM SUS

APPROVAL

PART NAME

CUSTOM CABLE SPECIFICATION V25G DESIGNER J. HEEFNER MAY/10/2012 SIZE DWG. NO. MAY/10/2012 D DRAFTER E. BROWN CHECKER

PROJECTION:

SHEET 1 OF 1

53in. 1346.2mm **NOT TO SCALE** PIN 1 **CONNECTOR**

DCN#

DRAWING TREE #

DATE

V25G CABLE ASSEMBLY CIRCUIT SUMMARY V-DB25 M/S1-53-μD25 F/S1								
CABLE NAME	COND WIRE ID	TWISTED PAIR	LENGTH	FROM	то			
V25G	25 COND. CABLE	(12 TOTAL)	53 in.	Conn. J1	Conn.			
C 1	SHIELD (COPPER BRAID)		53 in.	PIN 1, SHIELD & SHELL	PIN 1, SHIELD SHELL			
	W1	SINGLE WIRE	53 in.	PIN 1, SHIELD & SHELL	PIN 1, SHIELD SHELL			
	W2	TP-1	53 in.	PIN 2	PIN 2			
	W14	IF-I	53 in.	PIN 14	PIN 14			
	W3	TD O	53 in.	PIN 3	PIN 3			
	W15	TP-2	53 in.	PIN 15	PIN 1			
	W4	TP-3 TP-4	53 in.	PIN 4	PIN 4			
	W16		53 in.	PIN 16	PIN 1			
	W5		53 in.	PIN 5	PIN 5			
	W17		53 in.	PIN 17	PIN 17			
	W6	TP-5	53 in.	PIN 6	PIN 6			
	W18		53 in.	PIN 18	PIN 18			
	W7	TP-6	53 in.	PIN 7	PIN 7			
	W19	11 -0	53 in.	PIN 19	PIN 1			
	W8	TP-7	53 in.	PIN 8	PIN 8			
	W20		53 in.	PIN 20	PIN 20			
	W9	TP-8	53 in.	PIN 9	PIN 9			
	W21		53 in.	PIN 21	PIN 2			
	W10	TP-9	53 in.	PIN 10	PIN 10			
	W22		53 in.	PIN 22	PIN 2			
	W11	TP-10	53 in.	PIN 11	PIN 1			
	W23	11 - 10	53 in.	PIN 23	PIN 23			
	W12	TP-11	53 in.	PIN 12	PIN 12			
	W24	11 - 1 1	53 in.	PIN 24	PIN 24			
	W13	TP-12	53 in.	PIN 13	PIN 13			
	W25	11 -12	53 in.	PIN 25	PIN 25			

* THE LENGTH SHOWN IN THIS LIST IS THE LENGTH OF THE CABLE BETWEEN THE TWO CONNECTORS. ADD ADDITIONAL LENGTH AS NECESSARY FOR THE INTERNAL WIRING OF THE CONNECTORS AND STRIP LENGTH.

V-DB25 M/S1-53-μD25 F/S1 STANDARD USE FOR THIS CABLE **SUBSYSTEM** AIR/VAC STANDARD USE **QUAD SUSPENSION UIM** IN-VAC