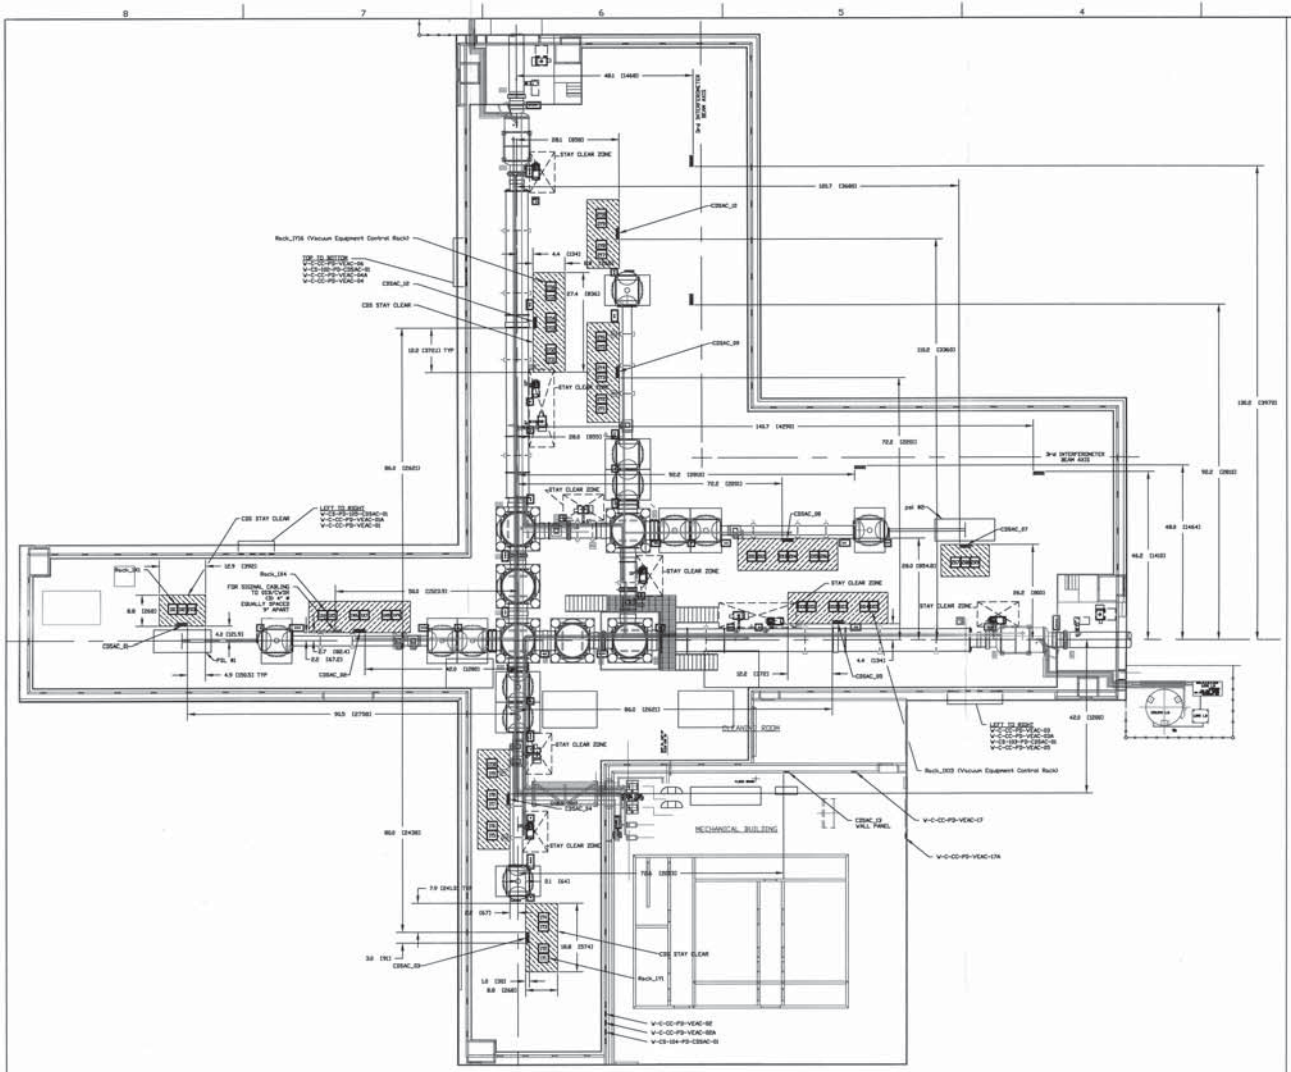

NOTES:

1. ANNULUS ION PUMPS ARE LOCATED ON THE CHAMBERS, NOT ON THE FLOOR AS SHOWN.
2. PORTABLE CLEAN ROOMS MUST FIT AROUND EACH CHAMBER (ONLY ONE SHOWN). LARGE CLEANROOM (FOR BSC CHAMBER) IS NOW 18'-7" SQ. (NOT 16' SQ. AS SHOWN).

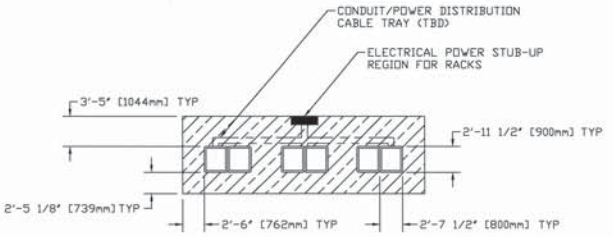

TYPICAL RACK CLUSTER ARRAINGEMENT

DWG. NO.	DESCRIPTION	DWG. NO.	DESCRIPTION
REFERENCE DRAWINGS			

UNLESS OTHERWISE SPECIFIED
DIMENSIONS ARE IN FEET (cm)
TOLERANCES:
FRACTIONAL ±
ANGULAR MACH ± BEND ±
TWO PLACE DECIMAL ±
THREE PLACE DECIMAL ±
FINISHED SURFACE RMS
BREAK CORNERS ON CUT:
REMOVE ALL BURRS

DO NOT SCALE THIS DRAWING
USED ON:
NEXT ASS'Y:

REV	DESCRIPTION	SYS	DET	CDS	VE	CC	BT	DRWN	DATE
00	INITIAL-RELEASE							CONLEY	09-20-96

ISSUE DESCRIPTION

LIGO CALIFORNIA INSTITUTE OF TECHNOLOGY MASSACHUSETTS INSTITUTE OF TECHNOLOGY

DETECTOR RACK LOCATIONS, LVEA-WA

CAD FILE	SIZE	DWG NO.	REV.
D961251-A-E.dwg	D	D961251-A-E	A
SCALE: NTS		SHEET: 1 OF 1	