

Title:

**SPECIFICATION FOR PIPING DESIGN AND MATERIAL**

**SPECIFICATION FOR  
PIPING DESIGN AND MATERIAL**

FOR

**LIGO VACUUM EQUIPMENT**

Hanford, Washington

And

Livingston, Louisiana

PROCESS ENGINEER: Robert Than

PROJECT ENGINEER: A. Moten

CIVIL/STRUC. ENGINEER: R. D. Watts

MANUFACTURING ENGINEER: Phillip F. Paul

QUALITY ASSURANCE ENGINEER: Alan D. Burdlock

PROJECT MANAGER: Paul Byg

JAN 22 1996

0	REL 1-19-96	D. M. W.	RELEASED FOR DESIGN & QUOTES DEO #0044
REV LTR.	BY-DATE	APPD. DATE	DESCRIPTION OF CHANGE
PROCESS SYSTEMS INTERNATIONAL, INC.			SPECIFICATION
INITIAL APPROVALS	PREPARED	DATE	APPROVED DATE
	R. Curtis	1-11-96	D. M. W. 1-18-96
			Number
			A V049-2-037
			LIGO-ES60008-00-V
			Rev.
			0

**TABLE OF CONTENTS**

1.0	SCOPE
2.0	CODES AND STANDARDS
3.0	MATERIAL/MANUFACTURING REQUIREMENTS
4.0	EXAMINATION AND TESTING
5.0	LINE NUMBER SYSTEM
6.0	VALVE AND INSTRUMENT NUMBERING SYSTEM
7.0	PIPING DESIGN AND MATERIAL SPECIFICATIONS
1B1	150# CLASS STAINLESS STEEL 304 - CRYOGENIC
1B2	150# CLASS STAINLESS STEEL 304 - NON-CRYOGENIC
C2	TYPE "L" COPPER TUBING - GENERAL NON-CRYOGENIC
T1	316 STAINLESS STEEL TUBING - CRYOGENIC
T2	304 STAINLESS STEEL TUBING - GENERAL NON-CRYOGENIC
T3	304L STAINLESS STEEL TUBING - VACUUM
T4	304L STAINLESS STEEL TUBING - ULTRA HIGH VACUUM
T5	304L STAINLESS STEEL TUBING - CLASS 100 CLEAN AIR
VJ	304 STAINLESS STEEL - CRYOGENIC VACUUM JACKETED SEE SPEC. V049-2-016

ATTACHMENT A

LIGO QUALITY ASSURANCE SUMMARY

**SPECIFICATION**

Number

**A**

V049-2-037

Rev.

0

**1.0 SCOPE**

The following piping and material specifications define the piping and fittings to be used for the LIGO Vacuum Equipment.

**2.0 CODES AND STANDARDS****2.1 Priority of Codes and Standards**

Priority of documents shall be as follows:

1. Codes (highest priority)
2. This specification

**2.2 Applicable Codes and Standards**

ANSI - American National Standards Institute

- B31.3 Chemical Plant and Petroleum Refinery Piping (for process piping only)
- B31.5 Refrigeration Piping
- B36.19 Stainless Steel Pipe
- B16.5 Pipe Flanges and Flange Fittings

ASTM - American Society of Testing and Materials

- A380-88 Standard Practice for Cleaning and Descaling Stainless Steel
- E427-71(81) Standard Practice for Testing for Leaks Using the Halogen Leak Detector
- E493-73(80) Standard Practice for Testing for Leaks Using the Mass Spectrometer Leak Detector in the inside-Out Testing Mode
- E498-73(80) Standard Test Method for Leaks Using the Mass Spectrometer Leak Detector or Residual Gas Analyzer in the Tracer Probe Mode
- E499-73(80) Standard Methods of Testing for Leaks Using the Mass Spectrometer Leak Detector Probe Mode

**SPECIFICATION**

Number **A** V049-2-037

Rev. **2**

Page **3** of

**2.3 Specification Compliance**

The equipment shall comply with any drawings, data sheets, specifications, codes and standards (latest editions) referred to or attached as part of this specification. State or local codes or regulations, if applicable, will be provided as an attachment to this specification. The Vendor is responsible for compliance with such standards, specifications, codes and regulations, if attached.

**3.0 MATERIAL/MANUFACTURING REQUIREMENTS**


3.1 All materials used to manufacture the piping, tubing, flanges or fittings, as designated per this specification, are to be of U.S.A. origin and manufacture.

**4.0 EXAMINATION AND TESTING**

Examination and Pressure Testing as required by ANSI B31.3-1990 Chapter VI.

**5.0 LINE NUMBER SYSTEM**

4.1 Lines shall be numbered according to the following chart:

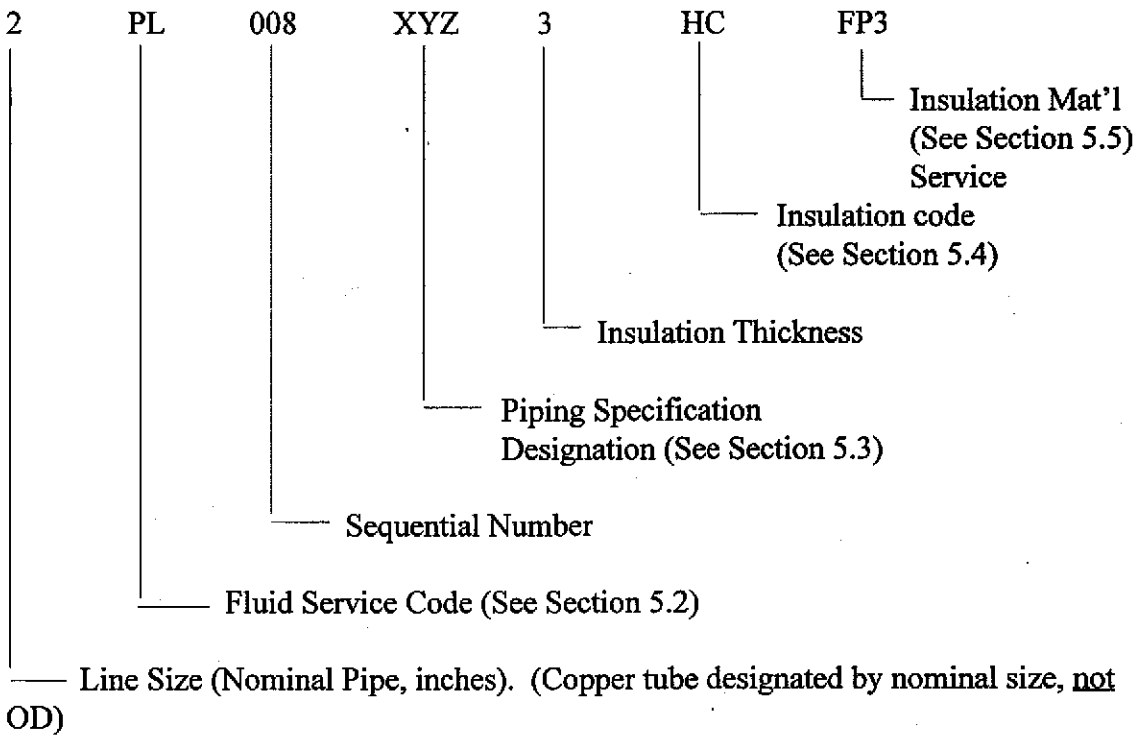

<b>SPECIFICATION</b>		
Number	A V049-2-037	Rev.
		0

Number  
Rev.

## 5.2 Fluid Codes

<u>Code</u>	<u>Fluid</u>
IA	Instrument Air
CA	Class 100 Clean Air
CWS	Cooling Water Supply
CWR	Cooling Water Return
NGS	Natural Gas Supply
LN2	Liquid Nitrogen
GN2	Gaseous Nitrogen
PV	Process Vacuum
PUV	Process Ultra High Vacuum
VA	Vent and Relief To ATM
N2	Nitrogen Gas
N	Nitrogen (Either Gas or Liquid)

## 5.3 Piping Specification Designation

4.4.1 "X" First Digit Identifiers

1 = 150 # ANSI

4.4.2 "Y" Second Digit Identifiers

A = 6061 T6 Aluminum  
 B = 304 Stainless Steel  
 C = Type L Copper Tubing  
 T = Stainless Steel Tubing

4.4.3 "Z" Third Digit Identifiers

1 = Cryogenic  
 2 = Non-Cryogenic  
 3 = Vacuum  
 4 = Ultra High Vacuum  
 5 = Class 100 Clean Air

## 5.4 Insulation Service

<u>Insulation Symbol</u>	<u>Insulation Service</u>
HC	Hot and Cold
C	Cold Conservation
PC	Personnel Protection COLD
PH	Personnel Protection HOT
VJ	Vacuum Jacketed

## SPECIFICATION

Number **A** V049-2-037Rev. **0**Page **5** of \_\_\_\_\_


**5.5 Insulation Material Codes**

FP3	1" Fiberglass Inner	2" Polyisocyanurate Outer
FP3.5	1" Fiberglass Inner	2 1/2" Polyisocyanurate Outer
FP4	1" Fiberglass Inner	3" Polyisocyanurate Outer

If no insulation material code appears in the line number then it shall be understood that no insulation is required.

**6.0 VALVE AND INSTRUMENT NUMBER SYSTEM**

Control valves, manual valves and associated instruments shall be designated according to P&ID Drawing Symbols. If the required designation is not specified on the drawing, then ISA-S5.1, Table 1 will take precedence.

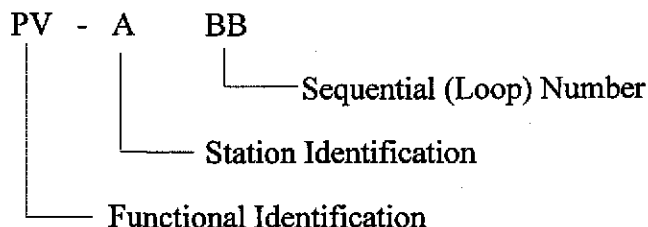

Manual valves that do not carry an instrument loop numbers (described above) shall be assigned one of the following valve type descriptions, preceded by the valve size in inches.

Type	Description
GVHV	Gate Valve, High Vacuum, SS, Viton Seals, Handwheel or Lever, CF Conn.
GVUH	Gate Valve, Ultra High Vacuum, SS, Viton Seals, Handwheel, CF Conn.
AVHV	Angle Valve, High Vacuum, SS, Viton Seals, Handwheel, ISOKF or K Conn.
AVUV	Angle Valve, Ultra High Vacuum, SS, Metal Seals, Handwheel, CF Conn.
IRV	Instrument Root Valve, SS
VJV	Vacuum Jacketed Valve, SS
BVCR	Ball Valve, Cryogenic, SS, 3 Piece
BVCA	Ball Valve, Class 100 Clean Air, SS, 3 Piece
GLV	Globe Valve
BVU	Ball Valve, Utility, Brass or Bronze
VSOV	Vacuum Seal-Off Valve, SS
VSOO	Vacuum Seal-Off Valve Operator, SS

**SPECIFICATION**

Number **A** V049-2-037

Rev. **0**

Title

**SPECIFICATION FOR PIPING DESIGN AND MATERIAL**

**1B1**

**PIPING DESIGN AND MATERIAL SPECIFICATION**

Service: Cryogenic

Primary Rating: 150# ANSI 304 SSTL

Design Conditions:

Pressure 0 to 192 psig

Temperature -320°F to 350°F

Corrosion Allowance Zero

Pipe:

12" and smaller ASTM A312 TP304

Pipe Schedule:

1 1/2" and smaller Schedule 10S SMLS

8" and smaller Schedule 10S SMLS or EFW

10" thru 12" Schedule 10S EFW

Note: Vacuum jacketed piping will be designed and fabricated in accordance with the manufacturer's standard, and PSI spec. V049-2-016.

Fittings:

1 1/2" and smaller Socket Welded 3000#

2" and larger Butt Weld

ASTM A403 WP304 WPS, WPW

O'Let's ASTM A182-F304

Flanges: Not allowed.

Valves: Valves shall be furnished under their own unique specification.

Continued on Next Page

Number  
Rev.

<b>SPECIFICATION</b>		
Number	V049-2-037	Rev.
<b>A</b>		<b>0</b>

Title

**SPECIFICATION FOR PIPING DESIGN AND MATERIAL**

**1B1**

Branch Connections:

Run  
Size "

½	04												04 - Tee
¾	06	04											05 - Sockolet
1	12	06	04										06 - Tee Then
1½	05	05	06	04									Reducer or
2	05	05	06	06	04								Reducing Tee
3	05	05	05	05	06	04							12 - BW O'let
4	05	05	05	05	12	06	04						
6	05	05	05	05	12	12	06	04					
8	05	05	05	05	12	12	12	06	04				
10	05	05	05	05	12	12	12	12	06	04			
12	05	05	05	05	12	12	12	12	12	06	04		
Branch Size	½	¾	1	1½	2	3	4	6	8	10	12		

**SPECIFICATION**

Number **A** V049-2-037

Rev. **0**

Page **5** of \_\_\_\_\_

Number

Rev.



Title

**SPECIFICATION FOR PIPING DESIGN AND MATERIAL**

**1B2**

**PIPING DESIGN AND MATERIAL SPECIFICATION**

Service: Non-Cryogenic - Clean

Primary Rating: 150# ANSI 304 SSTL

Design Conditions:

Pressure 0 to 192 psig  
Temperature -20>°F to 350°F  
Corrosion Allowance Zero

Pipe:

12" and smaller ASTM A312 TP304

Pipe Schedule:

1 1/2" and smaller Schedule 10S SMLS  
8" and smaller Schedule 10S SMLS or EFW  
10" thru 12" Schedule 10S EFW

Fittings:

1 1/2" and smaller Socket Welded 3000#  
2" and larger Butt Weld  
ASTM A403 WP304 WPS, WPW  
Elbow O'Let ASTM A182-F304

Flanges: 2" and larger ANSI 150# RF, ASTM A182 F304, Weldneck with o-ring gaskets.

Gaskets: O-ring, Viton non-lubricated, cleaned and sealed for shipment.

Valves: Valves shall be furnished under their own unique specification.

Continued on next page.

Number

Rev.

**SPECIFICATION**

Number **A** V049-2-037

Rev. **0**

Title

**SPECIFICATION FOR PIPING DESIGN AND MATERIAL**

1B2

Branch Connections:

Run  
Size "

½	04											04 - Tee
¾	06	04										05 - Sockolet
1	12	06	04									06 - Tee Then
1½	05	05	06	04								Reducer or
2	05	05	06	06	04							Reducing Tee
3	05	05	05	05	06	04						12 - BW O'let
4	05	05	05	05	12	06	04					
6	05	05	05	05	12	12	06	04				
8	05	05	05	05	12	12	12	06	04			
10	05	05	05	05	12	12	12	12	06	04		
12	05	05	05	05	12	12	12	12	12	06	04	
Branch Size	½	¾	1	1½	2	3	4	6	8	10	12	

Note:

1. Piping and fittings to be internally cleaned, dried and ends sealed during shipping, storing and installation.
2. ID of pipe and fittings to be free of hydrocarbon contamination, or dirt. of any kind.
3. Surface finish to be standard white pickled ID and O.D.
4. Tube Bending - The following is not allowed: Sand packing, Mechanical scratches on tube I.D., Any type of lubricant.
5. Material manufactures certificate of compliance to applicable ASTM specifications are required and must accompany shipment.
6. Tubing, flanges and fittings to be etched or stamped with manufacturers name, part number and material type.

Number

Rev.

**SPECIFICATION**

Number **A** V049-2-037

Rev. **0**

Title

**SPECIFICATION FOR PIPING DESIGN AND MATERIAL**

C2

**PIPING DESIGN AND MATERIAL SPECIFICATION**

Service: Gaseous Nitrogen, Cooling Water, Instrument Air

Design Conditions:

Pressure	200 PSIG
Temperature	-20°F to 150°F
Corrosion Allowance	Zero

Tube: All sizes Type "L" Copper - Hard Drawn ASTM B88, B280, Copper Tube designated by its Nominal sizes, not OD on P&ID's and piping drawings..

Note: Copper tube and fittings are to be specified on PSI BOM's by the actual O.D. of the tube.

Fittings: All sizes Wrought Copper ASTM B75  
All Fittings to be female solder cup ends.  
Brass Parker CPI tube fittings (or equal).

Unions: 1/4" to 1" Brass Parker CPI tube fittings (or equal) may also be used.

Valves: Valves shall be furnished under their own unique specification.

Soldering: All joints in wrought copper fittings shall be soldered using 95-5 Tin-Antimony.

Notes:

1. Tubing is to be internally cleaned and the ends sealed during shipping, storing and installation. Spools are to have all flux residue, grit, splatters or dirt removed before installation.
2. Fittings are to be cleaned after manufacturing and sealed in plastic during shipping, storing and installation.

Number  
Rev.

**SPECIFICATION**

Number **A** V049-2-037

Rev. **0**

Title

**SPECIFICATION FOR PIPING DESIGN AND MATERIAL**

**T1**

**PIPING DESIGN AND MATERIAL SPECIFICATION**

Service: Cryogenic

Design Conditions:

Pressure	0 to 300 psig
Temperature	-320°F to 350°F
Corrosion Allowance	Zero

Tube:

All sizes	ASTM A269 GR 304L SMLS Tube sizes designated by OD dimensions.
-----------	---

<u>Tube Size (OD):</u>	<u>Minimum Wall Thickness (Inches)</u>
------------------------	--

1/4"	0.035"
3/8"	0.035"
1/2"	0.049"
3/4"	0.049"
1"	0.065"

Fittings: All Fittings to be Parker Weld tube fittings SA479 or ASTM A276 GR TP316 and ASTM A182 GR TP316, or equal.

Valves: Valves shall be furnished under their own unique specification.

Note:

1. Tubing to be internally cleaned, dried and ends sealed during shipping, storing and installation. Tube ID to be free of hydrocarbon contamination.
2. Fittings to be cleaned after manufacturing and sealed in plastic bags during shipping, storing and installation.
3. Tubing surface finish to be standard white pickled I.D. & O.D.

Number

Rev.

**SPECIFICATION**

Number	V049-2-037
<b>A</b>	

Rev.	0
------	---

Title

# SPECIFICATION FOR PIPING DESIGN AND MATERIAL

T2

## PIPING DESIGN AND MATERIAL SPECIFICATION

Service: Non-Cryogenic

Design Conditions:

Pressure	0 to 300 psig
Temperature	-20°F to 350°F
Corrosion Allowance	Zero

Tube:

All sizes	ASTM A269 GR TP304 SMLS Tube sizes designated by OD dimensions.
-----------	--

<u>Tube Size (OD):</u>	<u>Minimum Wall Thickness (Inches)</u>
------------------------	--

1/4"	0.035"
3/8"	0.035"
1/2"	0.049"
3/4"	0.049"
1"	0.065"

Fittings: All Fittings to be Parker A-LOK tube fittings SA479 or ASTM A276 GR TP316 and ASTM A182 GR TP316 or equal.

Valves: Valves shall be furnished under their own unique specification.

Note:

1. Tubing to be internally cleaned, dried and ends sealed during shipping, storing and installation. Tube ID to be free of hydrocarbon contamination.
2. Fittings to be cleaned after manufacturing and sealed in plastic bags during shipping, storing and installation.
3. Tubing surface finish to be standard white pickled I.D. & O.D.

Number

Rev.

### SPECIFICATION

Number	V049-2-037
<b>A</b>	

Rev.	0
------	---

Title

**SPECIFICATION FOR PIPING DESIGN AND MATERIAL**

**T3**

**PIPING DESIGN AND MATERIAL SPECIFICATION**

**Service:** Process Vacuum

**Design Conditions:**

Pressure Vacuum  $10^{-5}$  Torr to 2 psig  
 Temperature -20°F to 150°F  
 Corrosion Allowance Zero

**Tube:** (Tube sizes designated by OD dimensions)

All sizes up to 1" ASTM A269 GR TP304L SMLS  
 1 1/2" and larger ASTM A26 GRTP304L SMLS or Welded.

<b>Tube Size (OD):</b>	<b>Minimum Wall Thickness (Inches)</b>	<b>Conflat Flange Size</b>	<b>No. Bolts</b>	<b>B.C. Dia.</b>	<b>Thru Hole Dia.</b>
1/4"	0.035"	1 1/3" Nom. O.D.	6	1.062"	.172"
3/8"	0.035"	1 1/3" Nom. O.D.	6	1.062"	.172"
1/2"	0.035"	1 1/3" Nom. O.D.	6	1.062"	.172"
3/4"	0.035"	2 1/8" Nom. O.D.	4	1.625"	.265"
1"	0.065"	2 3/4" Nom. O.D.	6	2.312"	.265"
1 1/2"	0.065"	2 3/4" Nom. O.D.	6	2.312"	.265"
2"	0.065"	3 3/8" Nom. O.D.	8	2.85"	.332"
2 1/2"	0.065"	4 1/2" Nom. O.D.	8	3.628"	.332"
4"	0.083"	6" Nom. O.D.	16	5.128"	.332"
6"	0.083	8" Nom. O.D.	20	7.128"	.332"
8"	0.120	10" Nom. O.D.	24	9.128"	.332"
10"	0.120	12" Nom. O.D.	32	11.181"	.332"
12"	0.120	14" Nom. O.D.	30	12.810"	.390"
14"	0.120	16 1/2" Nom. O.D.	36	15.310"	.390"

**Flanges:** All Flanges to be Conflat, ISO Large Flange or KF tube fittings 304L Stainless Steel.

Continued on next page.

**SPECIFICATION**

Number **A** V049-2-037

Rev. **0**

Number

Rev.

## T3

**Fittings:** All fittings to be 304L butt weld or flanged O.D. tube, wall thickness to match tube wall thickness listed above.

**Valves:** Valves shall be furnished under their own unique specification.

**Notes:**

1. Tubing to be internally cleaned, dried and ends sealed during shipping, storing and installation. Tube ID to be free of hydrocarbon contamination.
2. Fittings to be cleaned after manufacturing and sealed in plastic bags during shipping, storing and installation.
3. Tubing surface finish to be standard white pickled I.D. & O.D.
4. Tube Bending - The following is not allowed: Sand packing, Mechanical scratches on tube I.D., or any type of lubricant.
5. Material manufactures certificate of compliance to applicable ASTM specifications are required and must accompany shipment.
6. Tubing, flanges and fittings to be etched or stamped with manufacturers name, part number and material type.
7. Conflat flanges to be made from either electro slag remelt, vacuum remelt or cross forged material.

Number

Rev.

**SPECIFICATION**

Number

**A**

V049-2-037

Rev.

0

Page 15 of \_\_\_\_\_

Title

## SPECIFICATION FOR PIPING DESIGN AND MATERIAL

T4

## PIPING DESIGN AND MATERIAL SPECIFICATION

**Service:** Process Ultra High Vacuum

**Design Conditions:**

Pressure Vacuum  $10^{-10}$  Torr to 2 psig  
 Temperature -20°F to 150°F  
 Corrosion Allowance Zero

**Tube:** (Tube sizes designated by OD dimensions)

All sizes up to 1" ASTM A269 GR TP304L SMLS  
 1 1/2" and larger ASTM A269 GRTP304 SMLS or welded.

Tube Size (OD):	Minimum Wall Thickness (Inches)	Conflat Flange Size	No. Bolts	B.C. Dia.	Thru Hole Dia.
1/4"	0.035"	1 1/3" Nom. O.D.	6	1.062"	.172"
3/8"	0.035"	1 1/3" Nom. O.D.	6	1.062"	.172"
1/2"	0.035"	1 1/3" Nom. O.D.	6	1.062"	.172"
3/4"	0.035"	2 1/8" Nom. O.D.	4	1.625"	.265"
1"	0.065"	2 3/4" Nom. O.D.	6	2.312"	.265"
1 1/2"	0.065"	2 3/4" Nom. O.D.	6	2.312"	.265"
2"	0.065"	3 3/8" Nom. O.D.	8	2.85"	.332"
2 1/2"	0.065"	4 1/2" Nom. O.D.	8	3.628"	.332"
4"	0.083"	6" Nom. O.D.	16	5.128"	.332"
6"	0.083"	8" Nom. O.D.	20	7.128"	.332"
8"	0.120"	10" Nom. O.D.	24	9.128"	.332"
10"	0.120"	12" Nom. O.D.	32	11.181"	.332"
12"	0.120"	14" Nom. O.D.	30	12.810"	.390"
14"	0.120"	16 1/2" Nom. O.D.	36	15.310"	.390"

Continued on next page.

## SPECIFICATION

Number

A

V049-2-037

Rev.

0

Page 16 of

Number

Rev.



## T4

- Flanges: All Flanges to be Conflat, 304L Stainless Steel.
- Fittings: All fittings to be 304L butt weld or flanged O.D. tube. Wall thickness to match tube wall thickness listed above.
- Valves: Valves shall be furnished under their own unique specification. Valves whose seats form part of the UHV boundary shall be all metal.
- Cleaning: Surfaces exposed to vacuum shall be cleaned and protected by PSI approved procedures suitable for UHV service.

## Note:

1. Tubing to be internally cleaned, dried and ends sealed during shipping, storing and installation. Tube ID to be free of hydrocarbon contamination.
2. Fittings to be cleaned after manufacturing and sealed in plastic bags during shipping, storing and installation.
3. Tubing surface finish to be standard white pickled I.D. & O.D.
4. Material manufacturers Certificate of Compliance to applicable ASTM specifications are required and must accompany shipment.
5. Tubing, flanges and fittings to be etched or stamped with manufacturers name, part number and material type.
6. Conflat flanges to be made from either electro slag remelt, vacuum remelt or cross forged material.

Number

Rev.

## SPECIFICATION

Number	A	V049-2-037	Rev.	0
--------	---	------------	------	---

Page 17 of

Title

**SPECIFICATION FOR PIPING DESIGN AND MATERIAL**

**T5**

**PIPING DESIGN AND MATERIAL SPECIFICATION**

Service: Class 100 Clean Air

Design Conditions:

Pressure Vacuum to 2 psig  
 Temperature -20°F to 150°F  
 Corrosion Allowance Zero

Tube: (Tube sizes designated by OD dimensions)

All sizes up to 1" ASTM A269 GR TP304 SMLS  
 1 1/2" and larger ASTM A269 GRTP304 SMLS or Welded.

Tube Size (OD):	Minimum Wall Thickness (Inches)	Conflat Flange Size	No. Bolts	B.C. Dia.	Thru Hole Dia.
1/4"	0.035"	1 1/3" Nom. O.D.	6	1.062"	.172"
3/8"	0.035"	1 1/3" Nom. O.D.	6	1.062"	.172"
1/2"	0.035"	1 1/3" Nom. O.D.	6	1.062"	.172"
3/4"	0.035"	2 1/8" Nom. O.D.	4	1.625"	.265"
1"	0.065"	2 3/4" Nom. O.D.	6	2.312"	.265"
1 1/2"	0.065"	2 3/4" Nom. O.D.	6	2.312"	.265"
2"	0.065"	3 3/8" Nom. O.D.	8	2.85"	.332"
2 1/2"	0.065"	4 1/2" Nom. O.D.	8	3.628"	.332"
4"	0.083"	6" Nom. O.D.	16	5.128"	.332"
6"	0.083"	8" Nom. O.D.	20	7.128"	.332"
8"	0.120"	10" Nom. O.D.	24	9.128"	.332"
10"	0.120"	12" Nom. O.D.	32	11.181"	.332"
12"	0.120"	14" Nom. O.D.	30	12.810"	.390"
14"	0.120"	16 1/2" Nom. O.D.	36	15.310"	.390"

Continued on next page.

Number

Rev.

<b>SPECIFICATION</b>		
Number <b>A</b>	V049-2-037	Rev. <b>0</b>

## T5

Flanges: All Flanges to be Conflat tube fittings 304 Stainless Steel.

Fittings: All Fittings to be 304 butt weld or flanged O.D. tube. Wall thickness to match the tube wall thickness.

Valves: Valves shall be furnished under their own unique specification

Cleaning: Internal surfaces shall be cleaned and protected by PSI approved procedures suitable for Class 100 air service.

## Note:

1. Tubing to be internally cleaned, dried and ends sealed during shipping, storing and installation. Tube ID to be free of hydrocarbon contamination.
2. Fittings to be cleaned after manufacturing and sealed in plastic bags during shipping, storing and installation.
3. Tubing surface finish to be standard white pickled I.D. & O.D.
4. Material manufactures Certificate of Compliance to applicable ASTM specifications are required and must accompany shipment.
5. Tubing, flanges and fittings to be etched or stamped with manufacturers name, part number and material type.
6. Conflat flanges to be made from either electro slag remelt, vacuum remelt or crossforged material.

Number

Rev.

## SPECIFICATION

Number

A

V049-2-037

Rev.

0

Page 19 of

ATTACHMENT "A"  
LIGO QUALITY ASSURANCE REQUIREMENTS SUMMARY

LIGO VACUUM EQUIPMENT	VENDOR:					JOB NO.: V59049
EQUIPMENT: PIPE, TUBING & FITTINGS	VENDOR ENG. OFFICE:					DWG. NO.:
PSI P.O. NO:	VENDOR FACTORY:					SPECNO: V049-2-037
TESTING INSPECTION AND DOCUMENTATION RECORD	Submittal After P.O.	Witnessed by PSI	Approval by PSI	Copies Req'd for PSI Files	Record in Mfr's File	Remarks:
						Inspector:  Date:
VENDOR Q.A. PLAN			X	2	X	
CLEANING PROCEDURE			X	2	X	
PREP FOR SHIPMENT PROCEDURE			X	2	X	
CERTIFICATE OF COMPLIANCE				2	X	

*Fig. 20.* SPEC V049-2-037