



Photon pressure induced test mass deformation




Stefan Hild (AEI Hannover)
LSC/Virgo meeting, March 2007, Det-Char-session

LIGO-G070173-00-Z

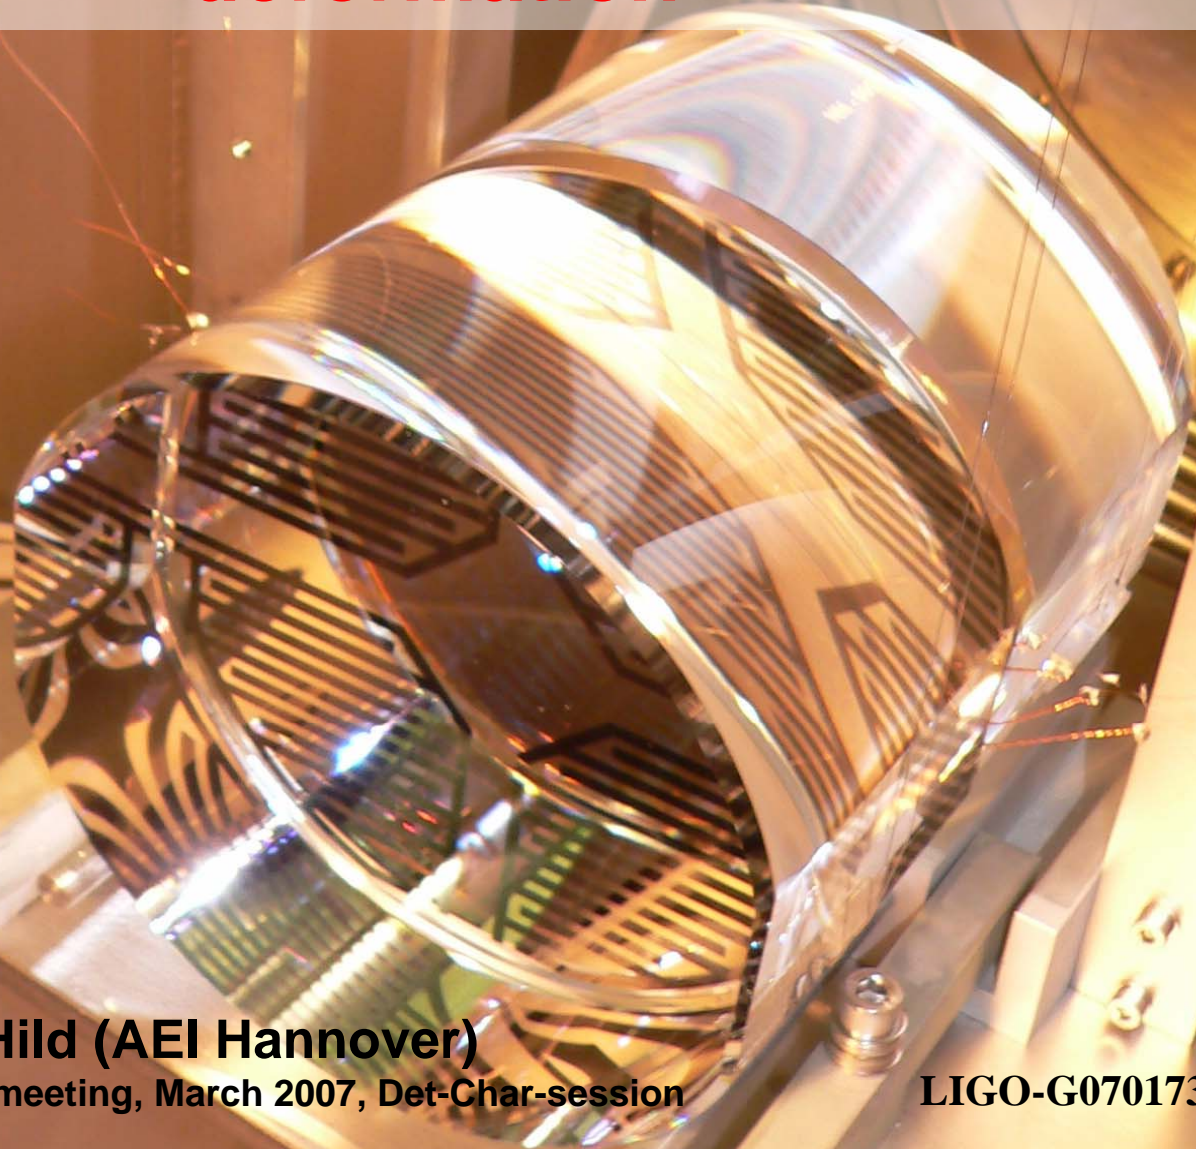


The GEO setup

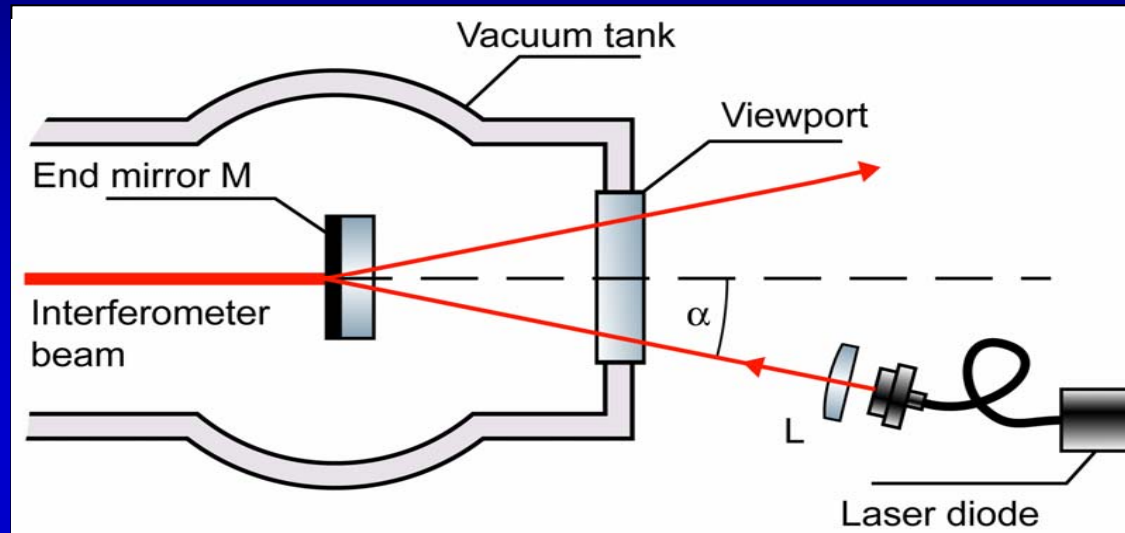

- Source: modulated Laser diode.
- Wavelength = 1035 nm, DC power = 1 W, modulated power up to 800 mW.
- Power is monitored by an photodiode inside the Laser diode.
- Shining from back (through the substrate)
- Restricted geometrical setup: the reflected beam is clipped on the way out of the vacuum.
- PPD beam diameter at MFN = 5mm (main IFO beam = 50 mm)




Pure PCAL response (without test mass deformation)

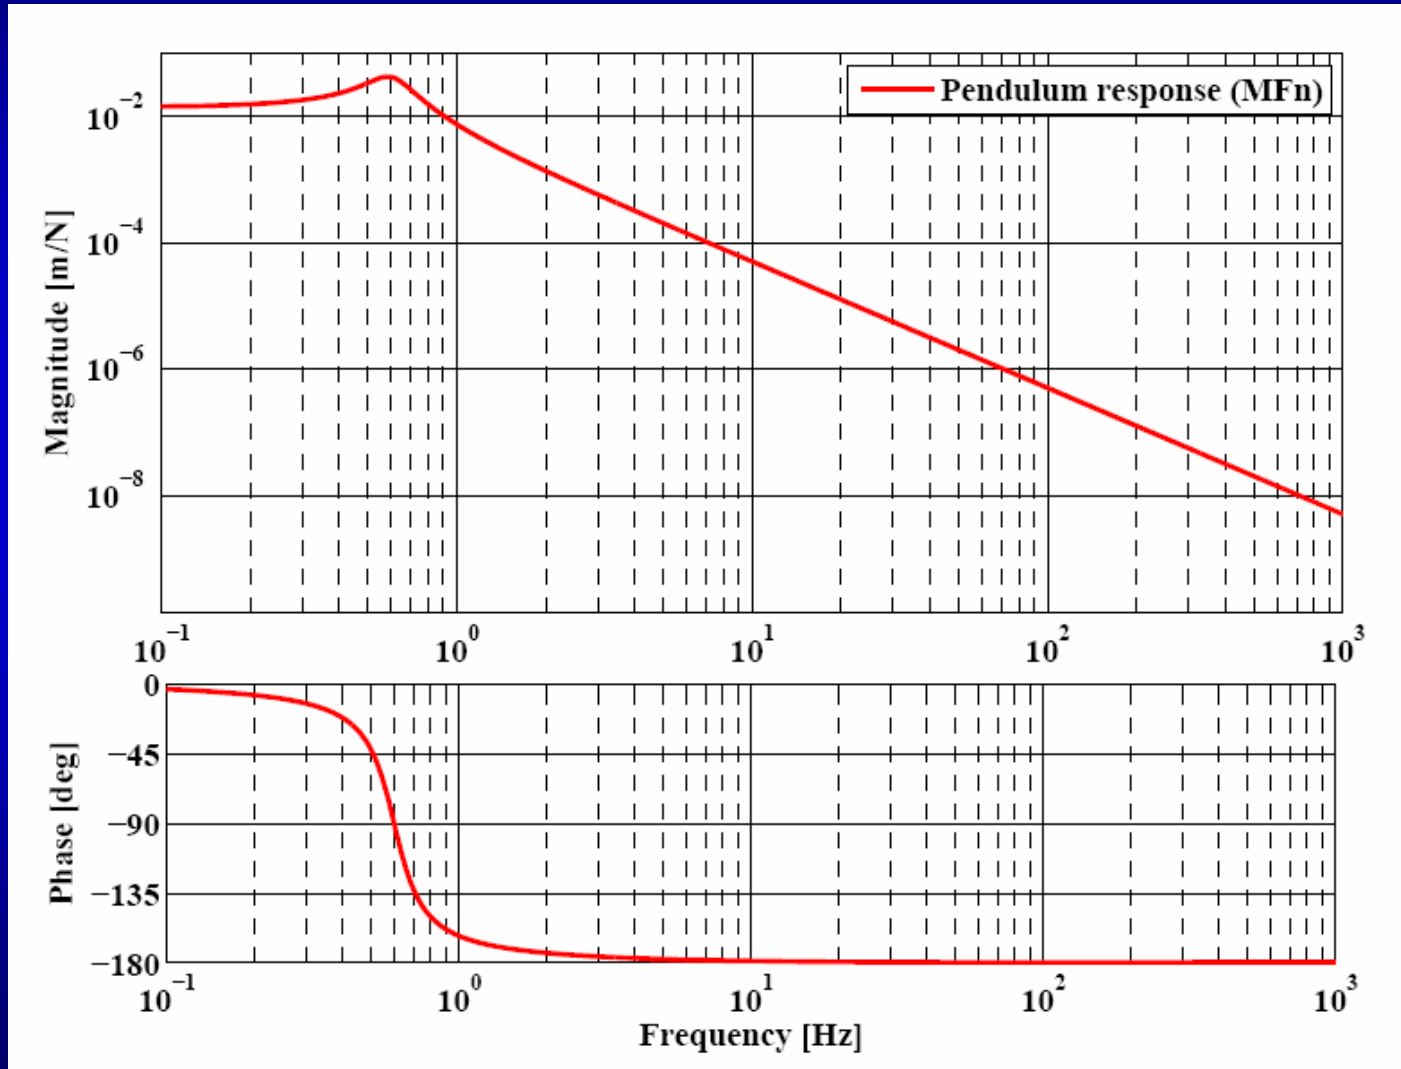



Comparison of official and photon pressure calibration

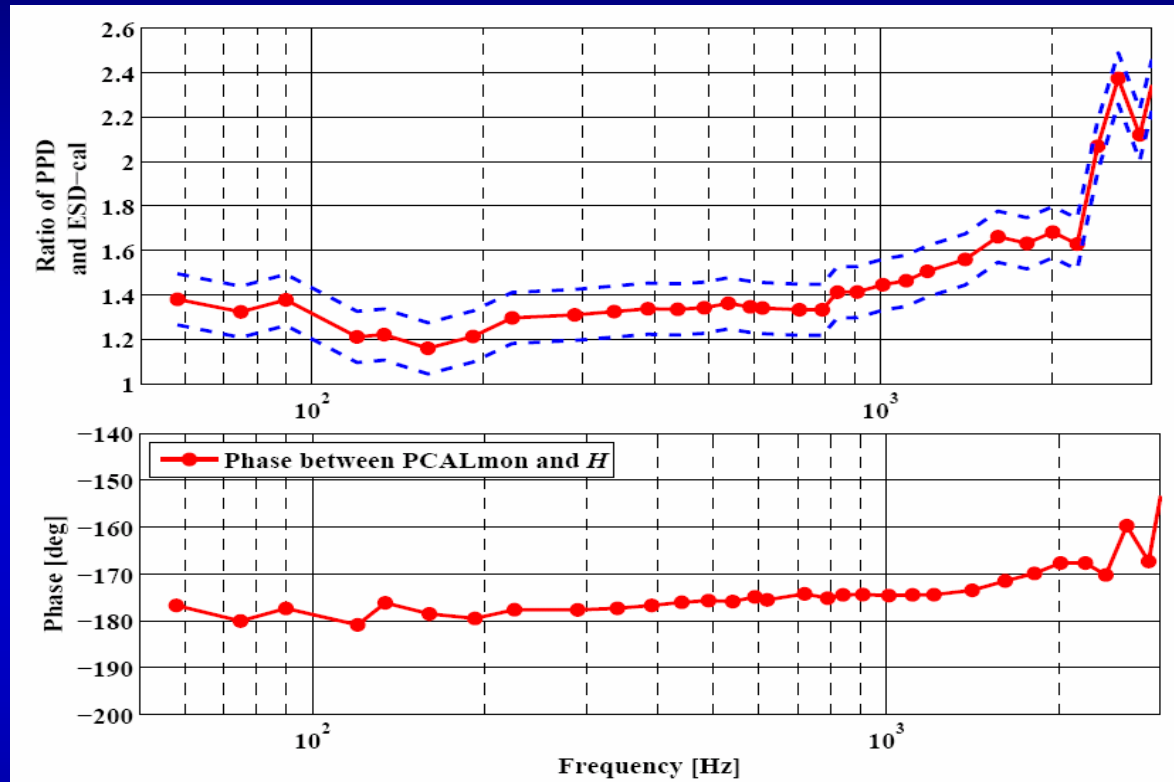


- Below 1kHz a systematic deviation of 30-40% is observed.
- Above 1kHz the deviation increases strongly
- In the following I will focus on the high frequency behaviour and explain it.



Finite element model




- Simulating the DC effect of radiation-pressure-induced test mass deformation.

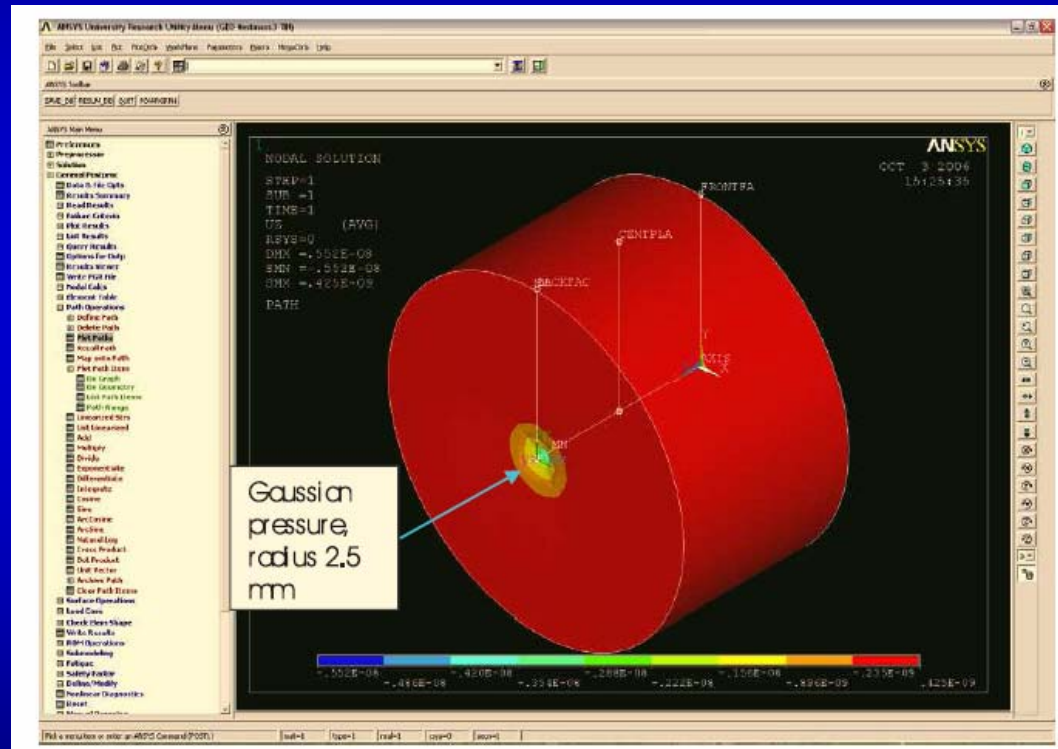

(Simulation was provided by our colleagues from Glasgow: I. Martin, S. Reid, J. Hough)



Effective displacement caused by mirror deformation

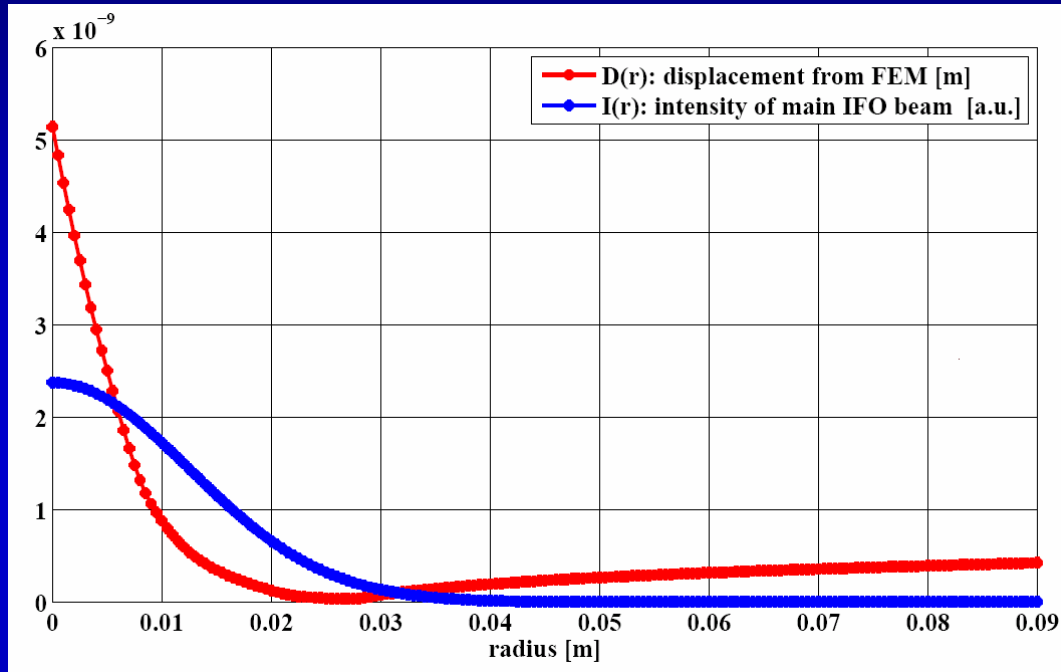

$$D_{\text{total}} = \int_0^{0.09\text{m}} \int_0^{2\pi} D_{\text{eff}} \cdot dr \cdot d\varphi = \int_0^{0.09\text{m}} 2\pi \cdot r \cdot k_I \cdot I(r) \cdot D(r) \cdot dr.$$

$$\int_0^{0.09\text{m}} 2\pi \cdot r \cdot k_I \cdot I(r) \cdot dr = 1.$$

- The effective mirror deformation amounts to $2.73 \times 10^{-10} \text{ m} / \text{N}$


Simple model

Assumptions:

- Below the internal resonances (<10 kHz) the mirror deformation is flat in frequency.
- Below the internal resonances the mirror deformation is in phase with the modulated light.
- The pendulum response is 180 degrees out of phase.

Prediction:

- Presence of a notch at the crossover of the responses from pendulum and mirror deformation.

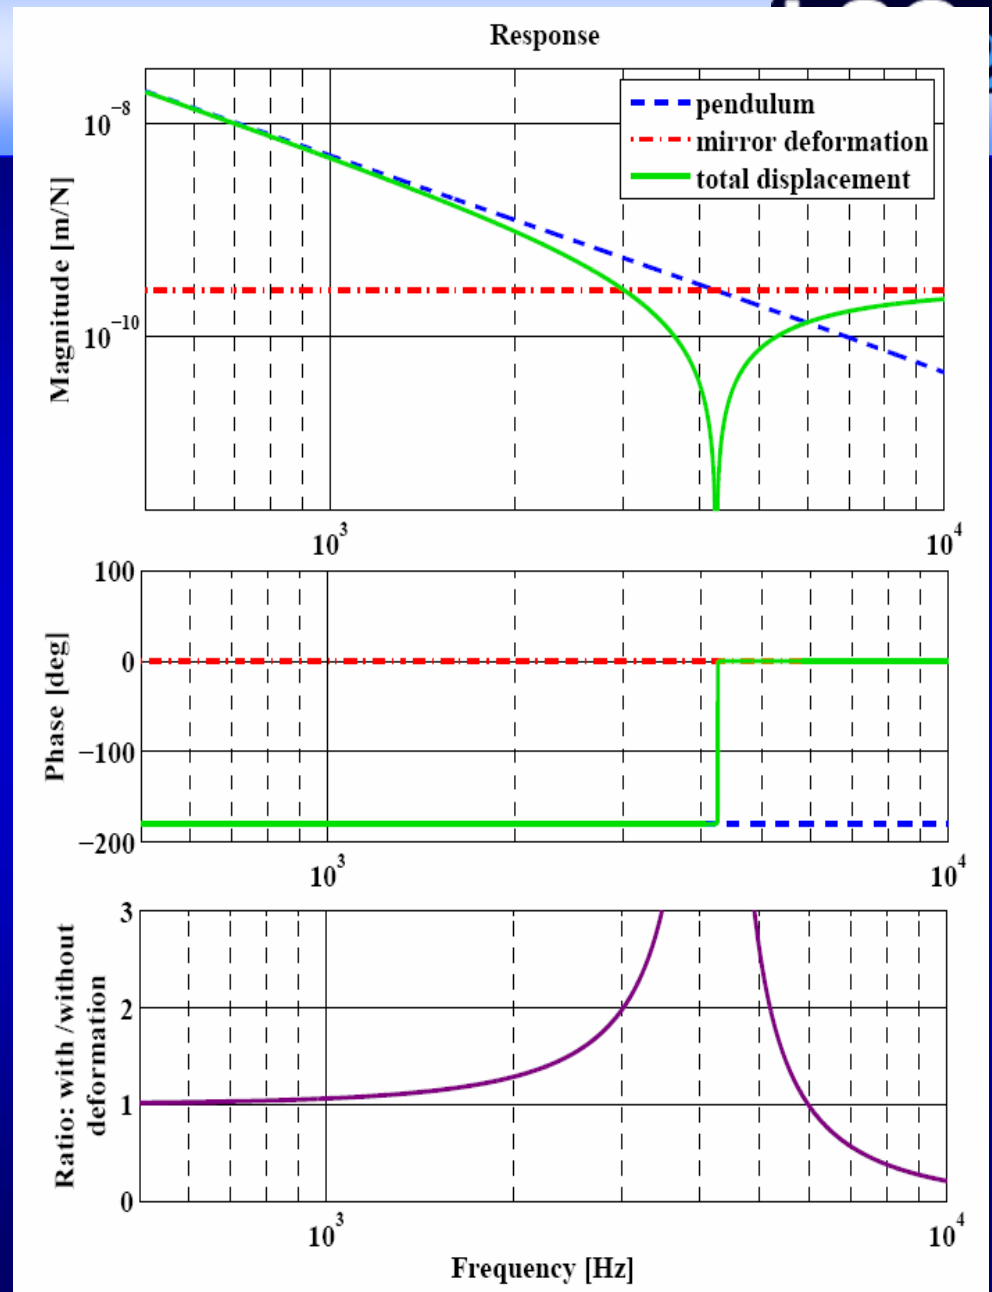


Transfer function of modulated light to the GW-channel at high frequencies



- Long duration measurements have been carried out at frequencies between 3 and 6kHz.
- Using a heterodyne downsampling technique up to 10 hours of data are used for a single DFT.

$$E_{\text{sig}} \cdot \sin(\omega_{\text{sig}}t) \cdot \sin(\omega_{\text{het}}t) = \frac{1}{2}E_{\text{sig}}[\cos(\omega_{\text{sig}} - \omega_{\text{het}})t - \cos(\omega_{\text{sig}} + \omega_{\text{het}})t]$$

- Presence of the notch was confirmed.
- Notch structure seems to be smeared out.

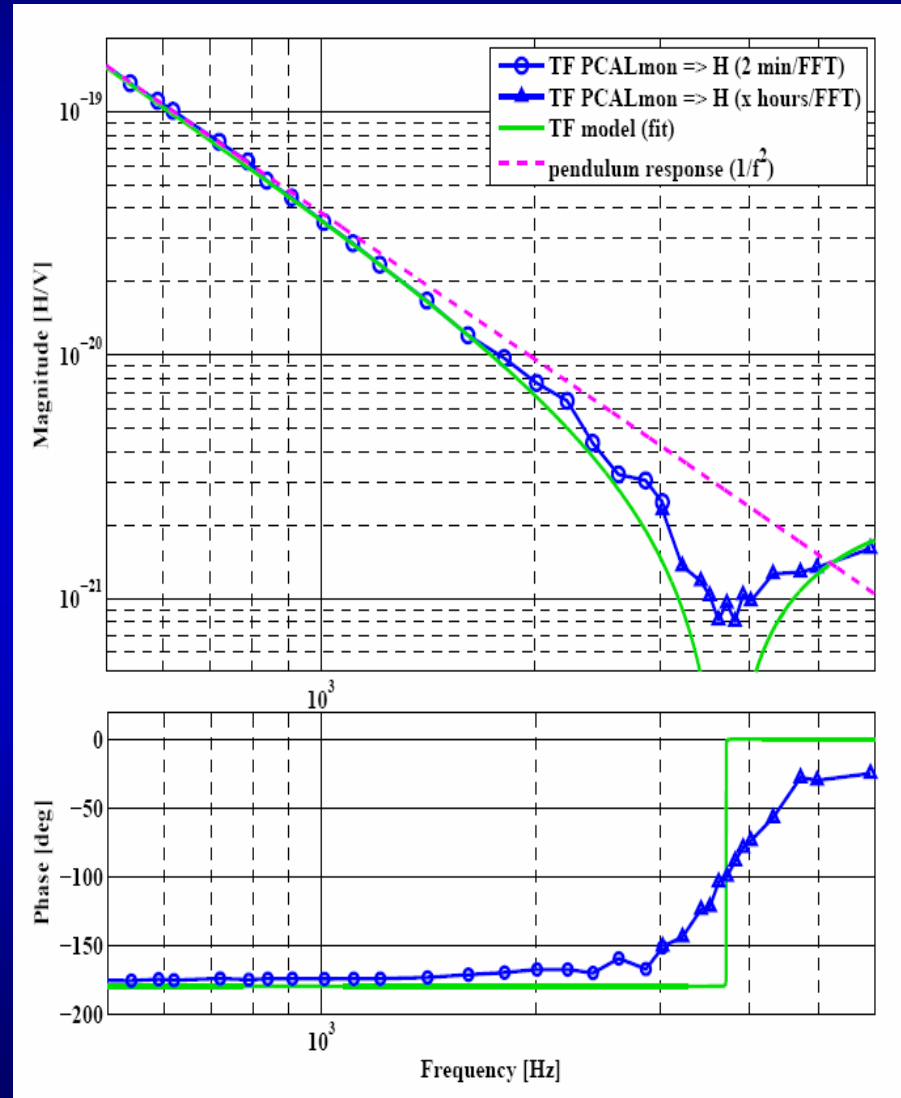




Explanation for the smearing-out of the notch: Jitter of the main IFO beam.



- Effective displacement seen by GEO600 depends on overlap of mirror deformation and main IFO beam:


$$D_{\text{total}} = k_I \int_0^{0.09\text{m}} \int_0^{360\text{deg}} \cdot I(r, \varphi) \cdot D(r, \varphi) \cdot dr \cdot d\varphi.$$

- The natural movement of the IFO beam can explain a shift of the notch frequency by several 100 Hz.
- The long duration measurements average over different notch frequencies.

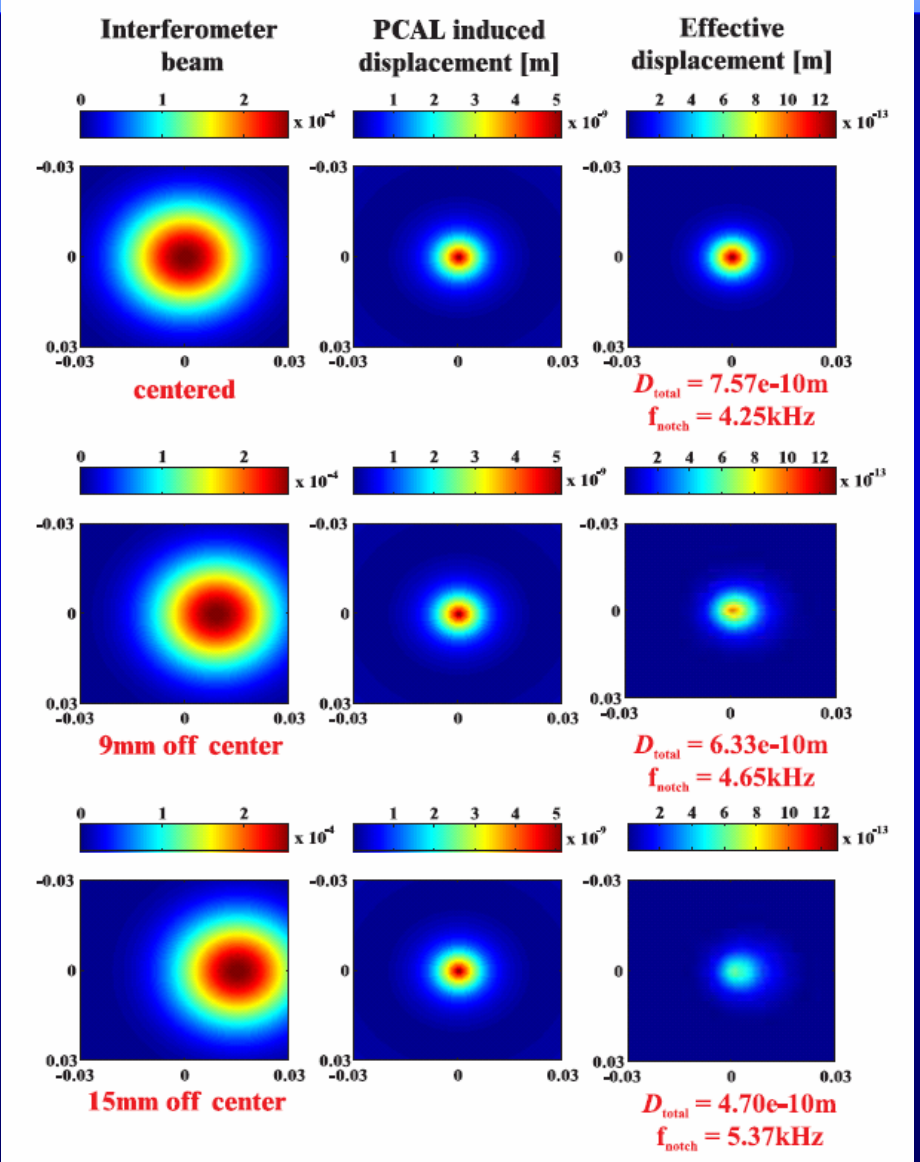



Explanation for the smearing out of the notch: Jitter of the main IFO beam.

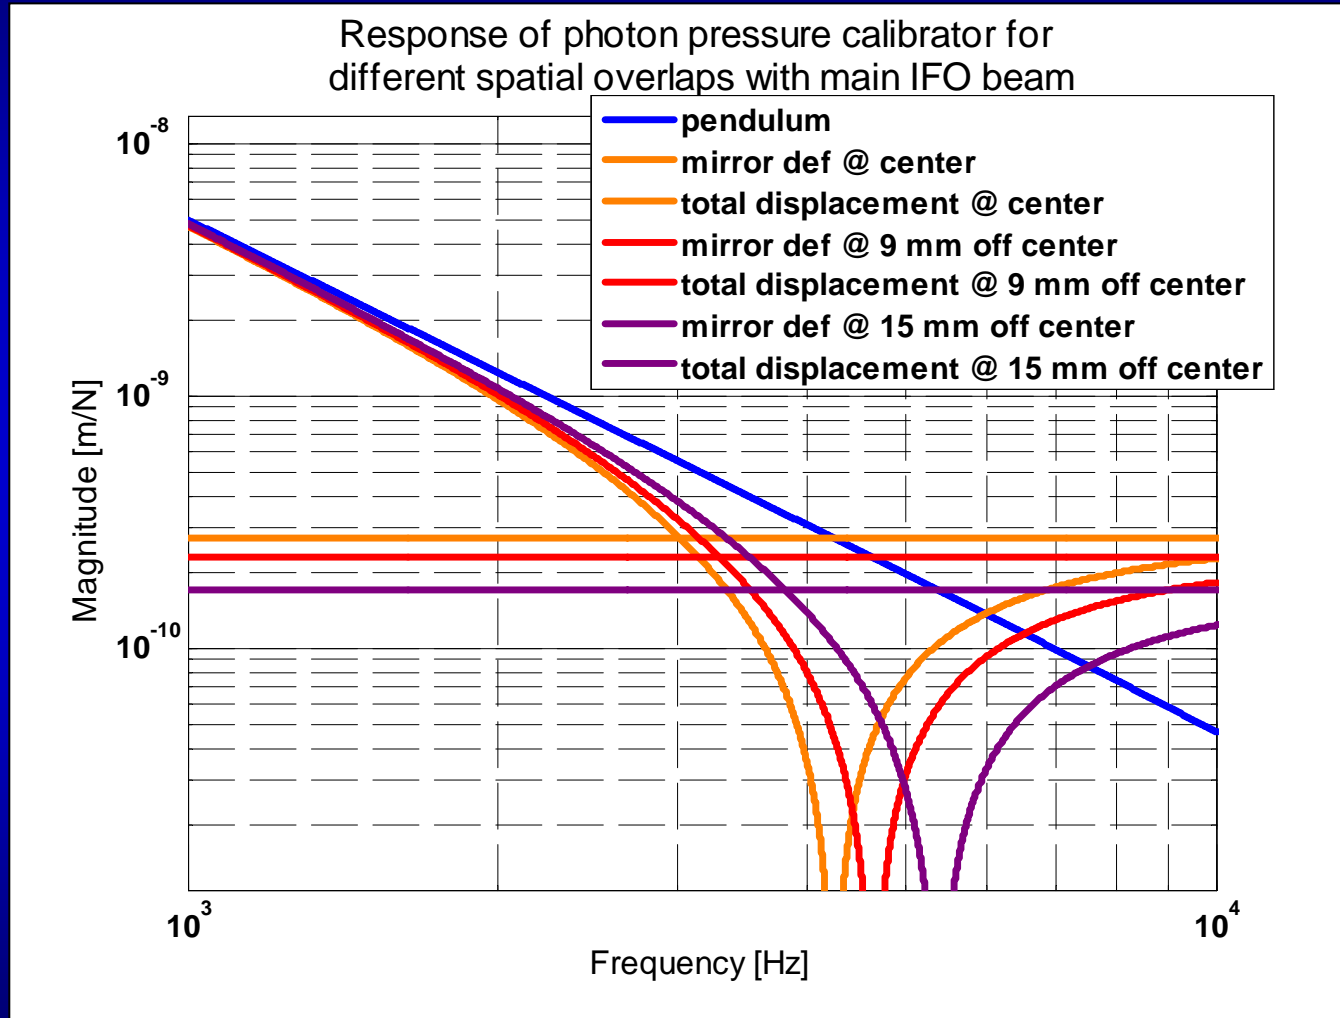



Summary of photon-pressure-induced testmass deformation





- Photon-pressure-induced mirror deformation limits the accuracy of the GEO photon pressure calibration above 1 kHz.
- Above 4 kHz this is the dominating effect.
- The test-masses are not rigid bodies !!
- Consequences:
 - At least at high frequencies the accuracy achievable with a photon pressure calibration is limited.
 - Coil/magnet actuators probably also cause a test mass deformation.
 - The mirror deformation might be reduced by applying a homogeneous actuation (for instance with an ESD).



END




Ruling out any artefacts from calibration process: Checking the $1/f^2$ of ESD vs official calibration.

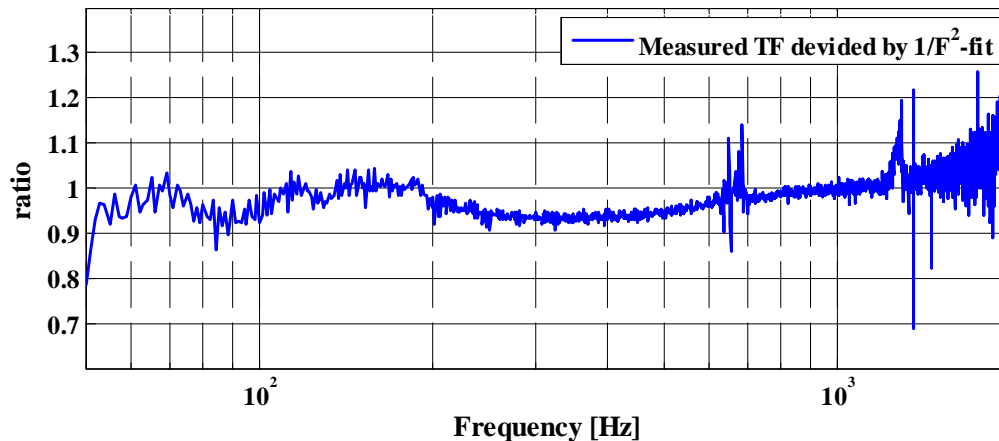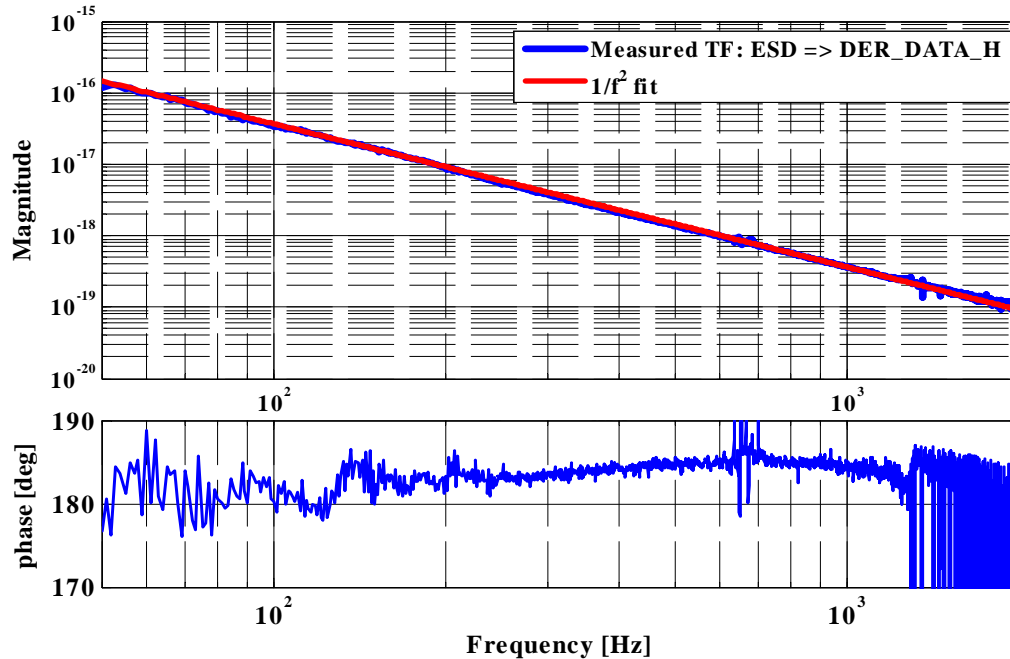

TF from ESD-FB to
DER_DATA_H is
 $1/f^2$ within +/-5%



Gravity calibrator

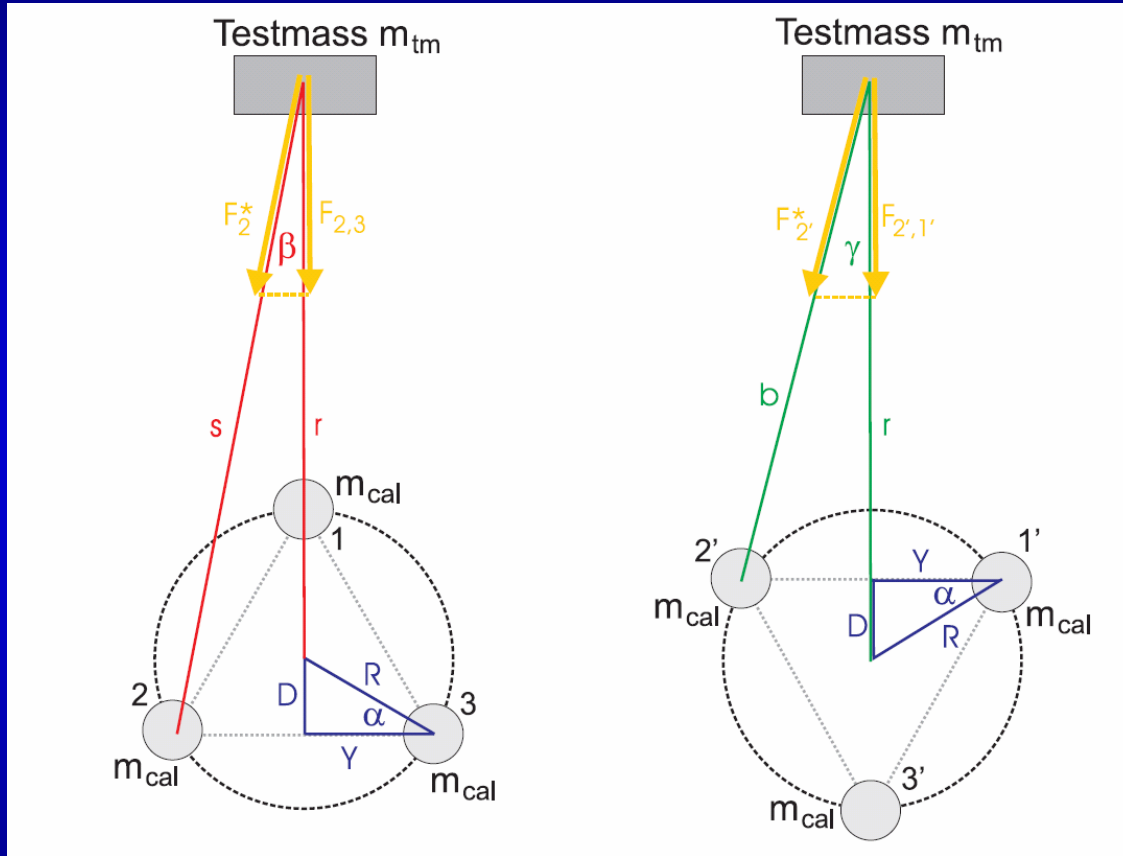

$$\Delta F = G \cdot m_{tm} \cdot m_{cal} \left[\frac{1}{(r + R)^2} + \frac{2 \cos \beta}{r^2 - rR + R^2} - \frac{1}{(r - R)^2} - \frac{2 \cos \gamma}{r^2 + rR + R^2} \right]$$

privileg Bild vergrößern


Wäscheschleuder

€ 149.95 B-Nr. 125240 G

[in den Warenkorb legen!](#)



Optical layout of the photon pressure calibrator

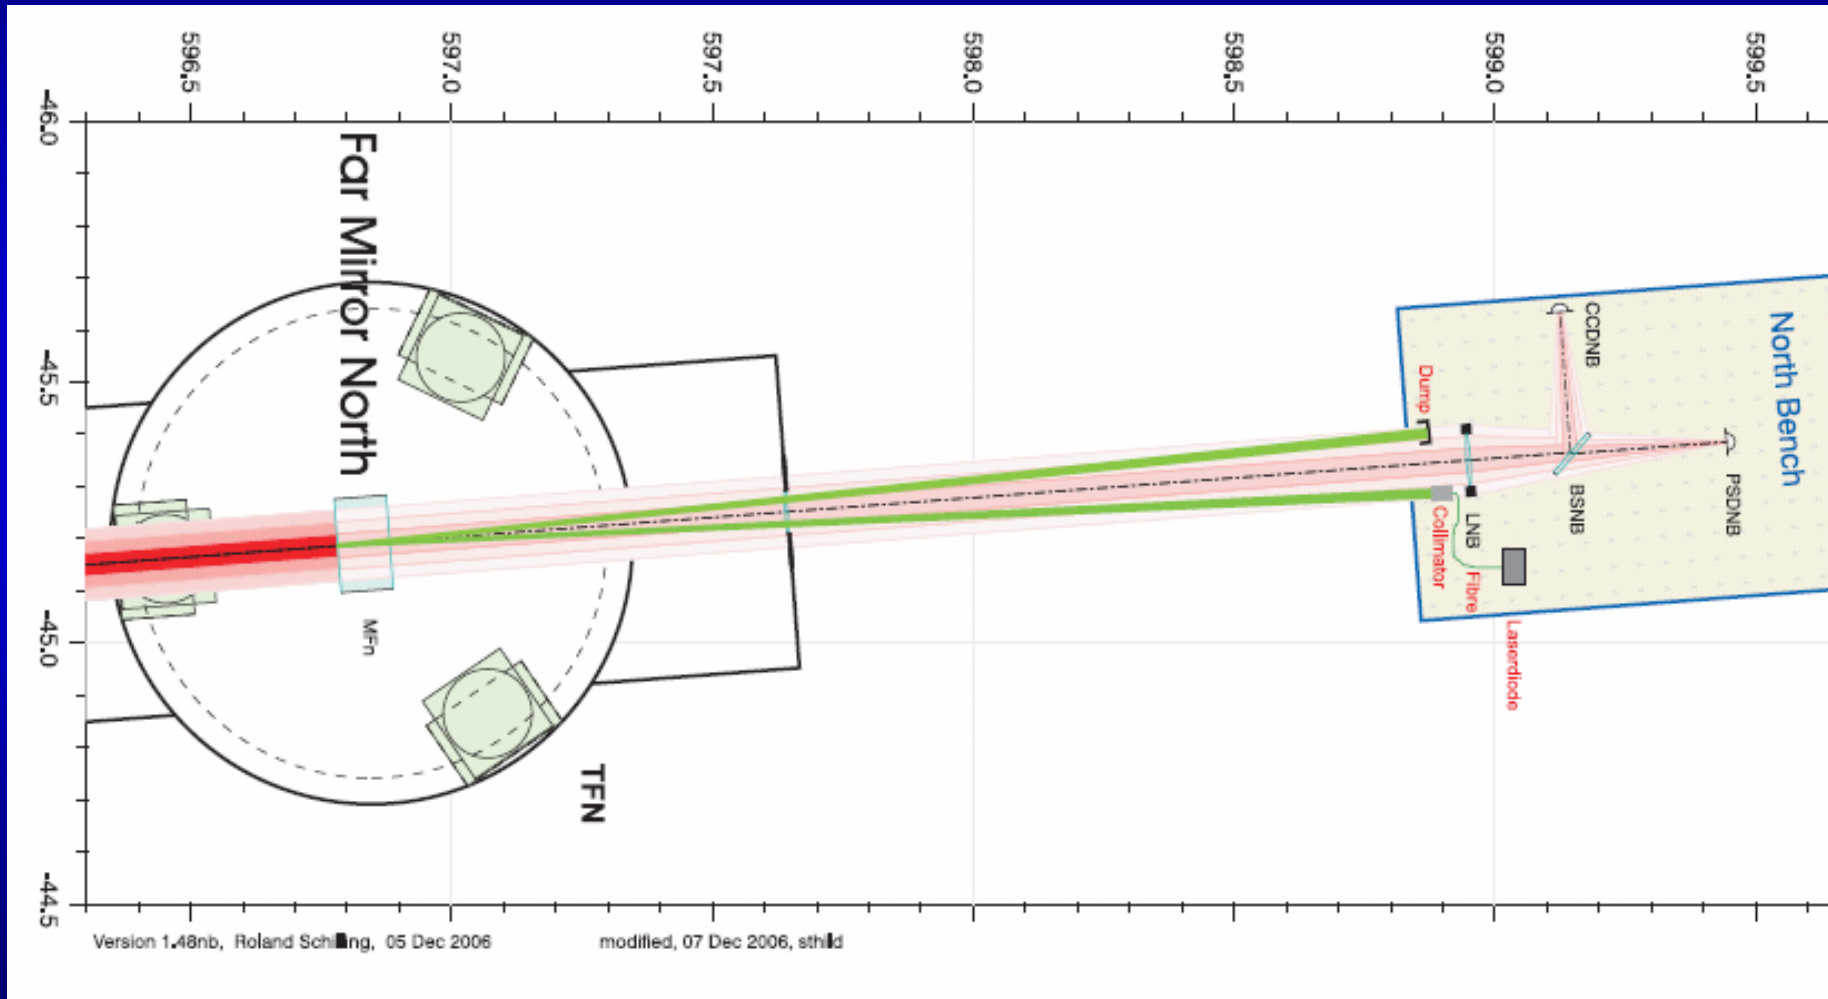



Effect from off-center laser beams

