


TCS cable route to/from field racks

Cables routed below the chamber

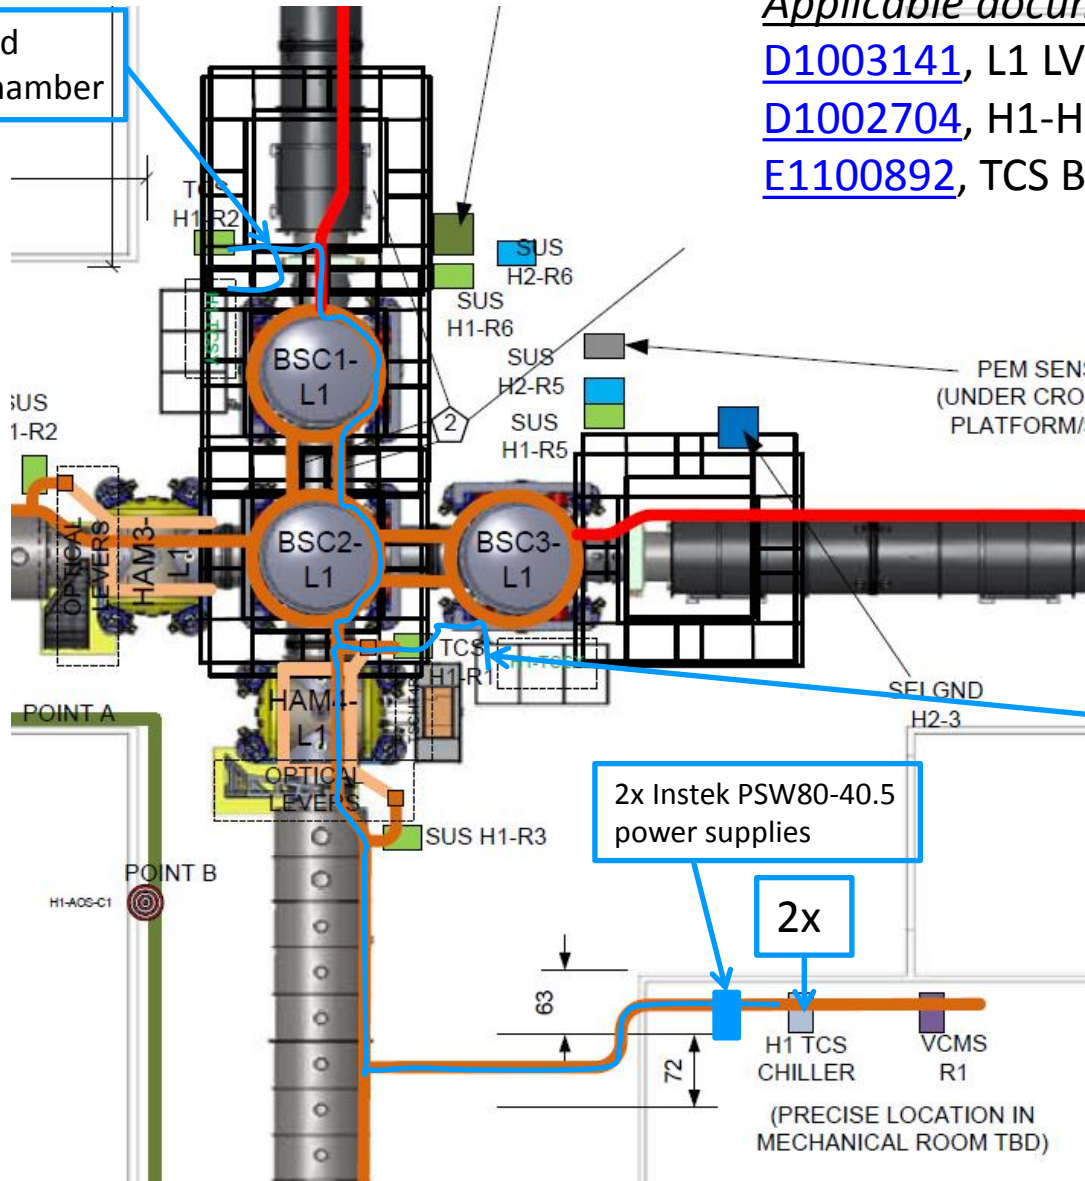

Applicable documents:

[D1003141](#), L1 LVEA layout

[D1002704](#), H1-H2 LVEA layout

[E1100892](#), TCS Block Diagram

Cables routed below the chamber

2x Instek PSW80-40.5 power supplies

2x

H1 TCS CHILLER VCMS R1
(PRECISE LOCATION IN MECHANICAL ROOM TBD)