



COC QA TEST REPORT

ETM08 HR Coating Absorption

Test Date	April 19-20, 2013		
Author(S)	Liyuan Zhang, Margot Phelps, GariLynn Billingsley		
Approval(s)			
Specification Doc.	LIGO-E0900068	Specification	< 0.5 ppm
Procedure Doc.	LIGO-E1000863	Mean ± Error	0.3 ± 0.1
Conclusion	Qualified.		

Discussions and Comments:

Four radial scans were carried out along X+- and Y+- with the arrow of barrel at Y+ direction, as shown in Fig.1. The calibration was done by a contamination cavity HR mirror (1" in dia.), of which the HR absorption was measured to be 0.6 ppm in the optical contamination test.



ETM08 HR Coating Absorption

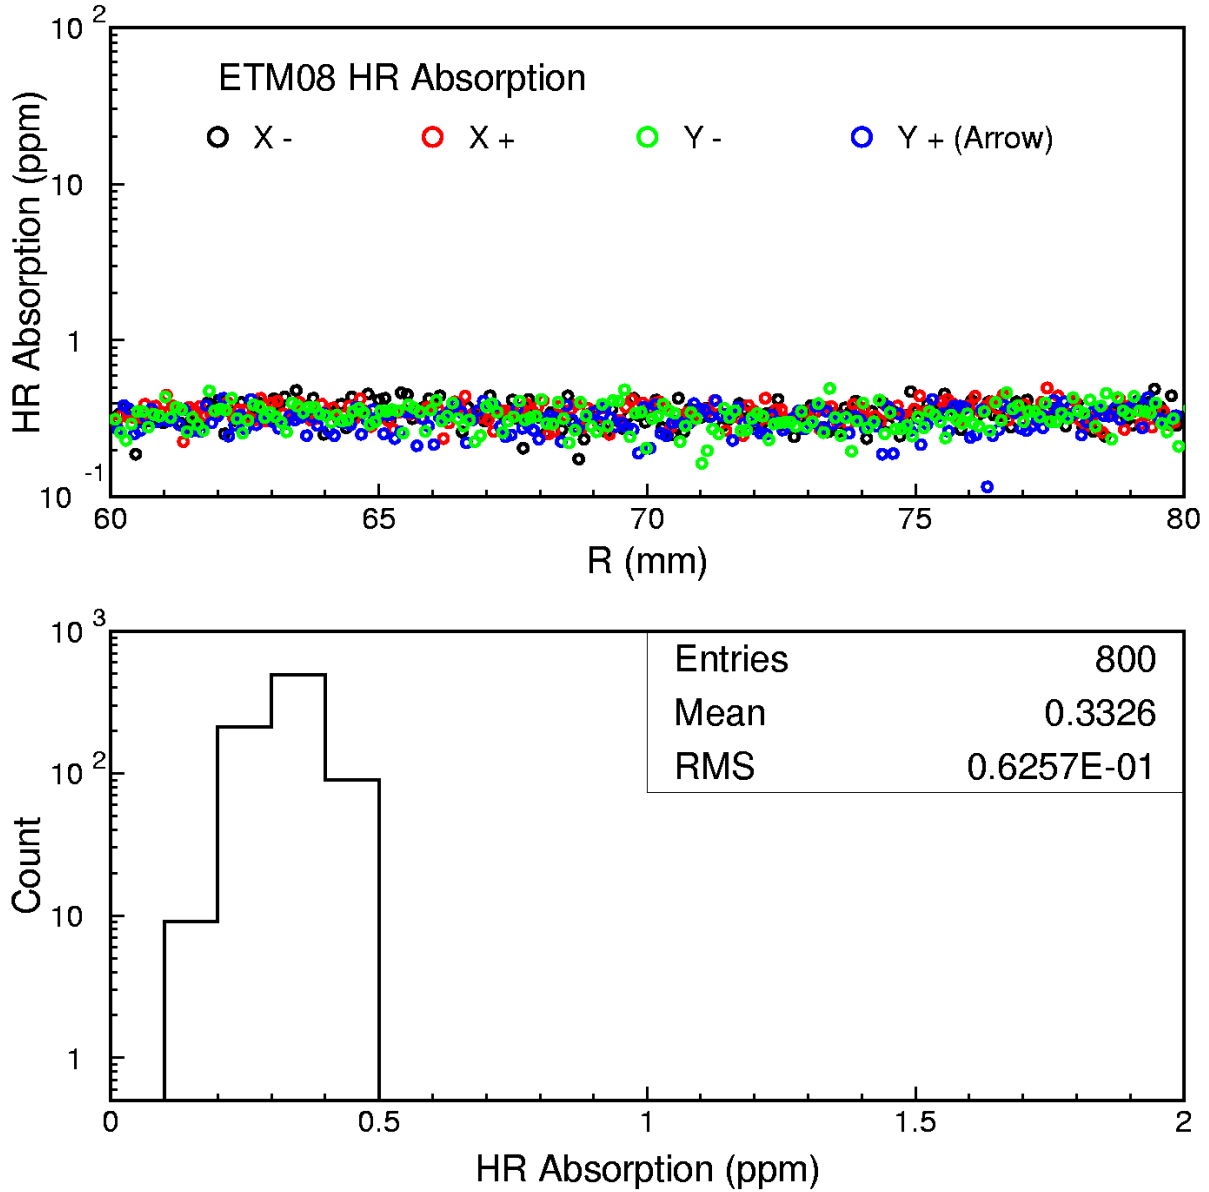


Fig.1 ETM08 HR absorption radial scans along 4 directions outside 120 mm aperture.