



## ETM12 AR Reflection

Test Date	May 23-24, 2013		
Author(S)	Liyuan Zhang, Margot Phelps, GariLynn Billingsley		
Approval(s)			
Specification Doc.	LIGO-E0900068	Specification	< 500 ppm
Procedure Doc.	LIGO-E1000863	Mean $\pm$ Error*	830 $\pm$ 10 ppm
Conclusion			

\* Error is the calibration error, which is ~1%.



### Discussions and Comments:

The scan was carried out over aperture of 160 mm in diameter with the beam and step sizes of 1 mm. The calibration is done by normalizing the AR reflection signal to the signal with a 1" HR mirror (T=70 ppm) and the variation of power during scan is monitored and corrected, the result is summarized in Fig.1.

The shallow fringes seem to be caused by interference between the AR reflection and the tail of strong reflection of HR. Since the wedge angle is only 0.07~0.1° (D080658), the separation of the two beam was not large enough at the measurement.



### ETM12 AR Reflection

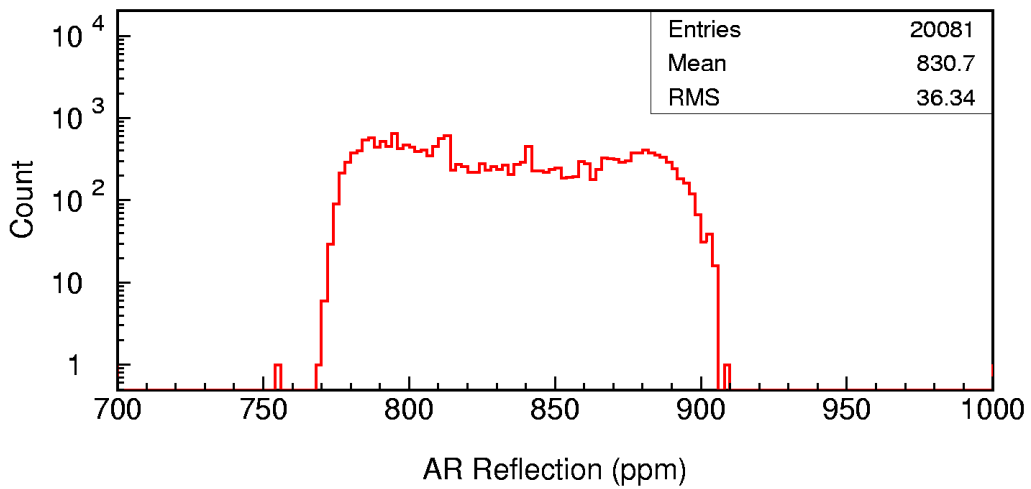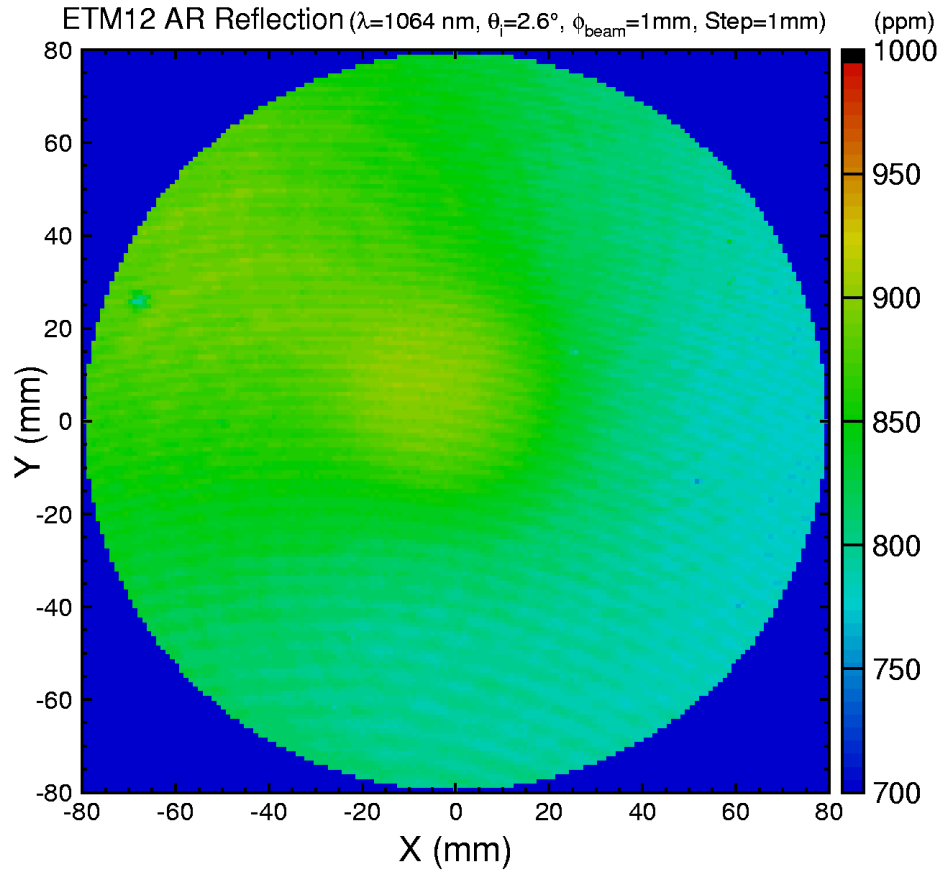

**Fig. 1 ETM12 S2 AR reflection over an aperture of 160 mm in diameter.**