



ITM09 PA test, after FC cleaning

Point-a

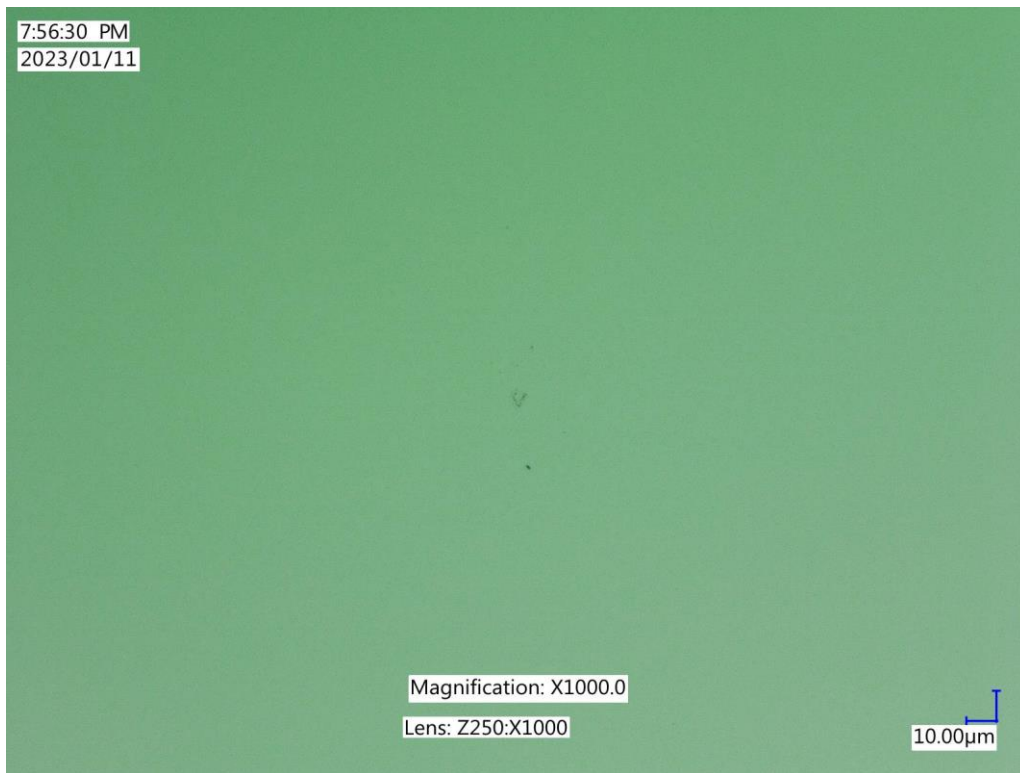


ITM09 point-b

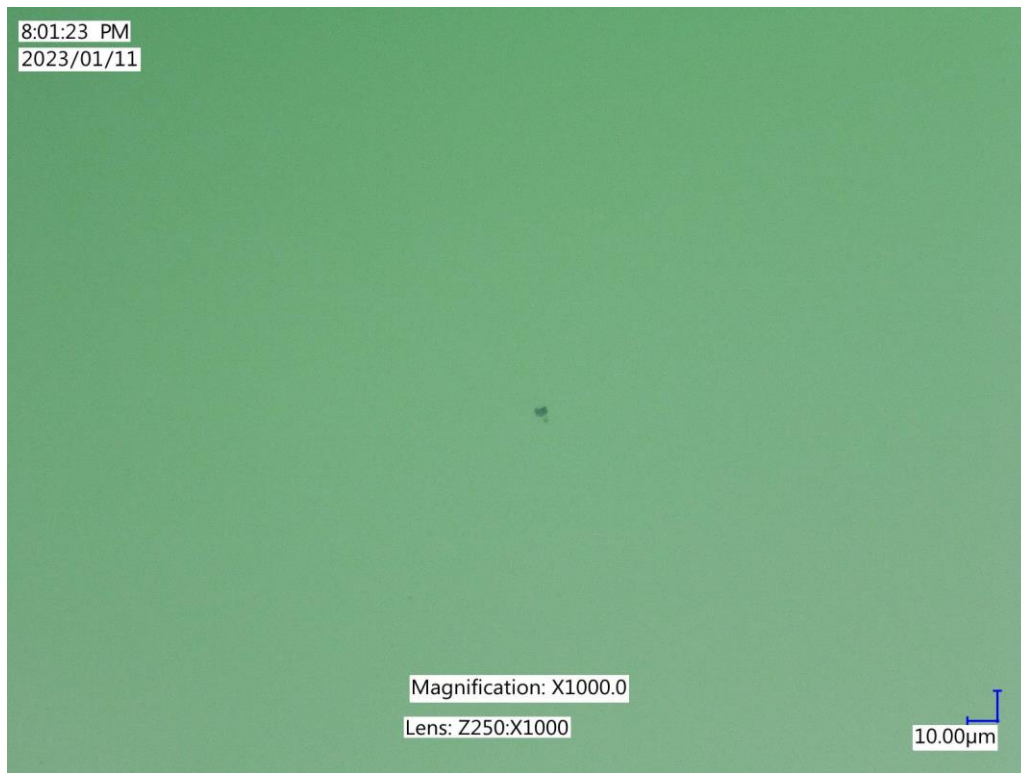



ITM09 point-c



ITM09 point-d

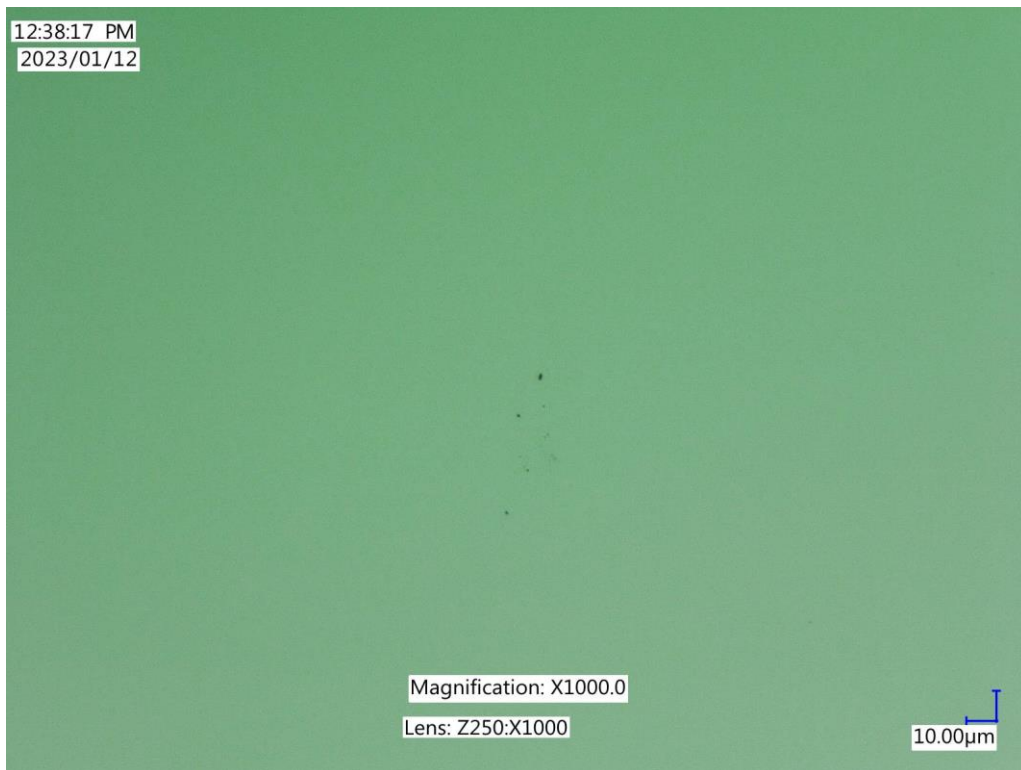

ITM09 point-e

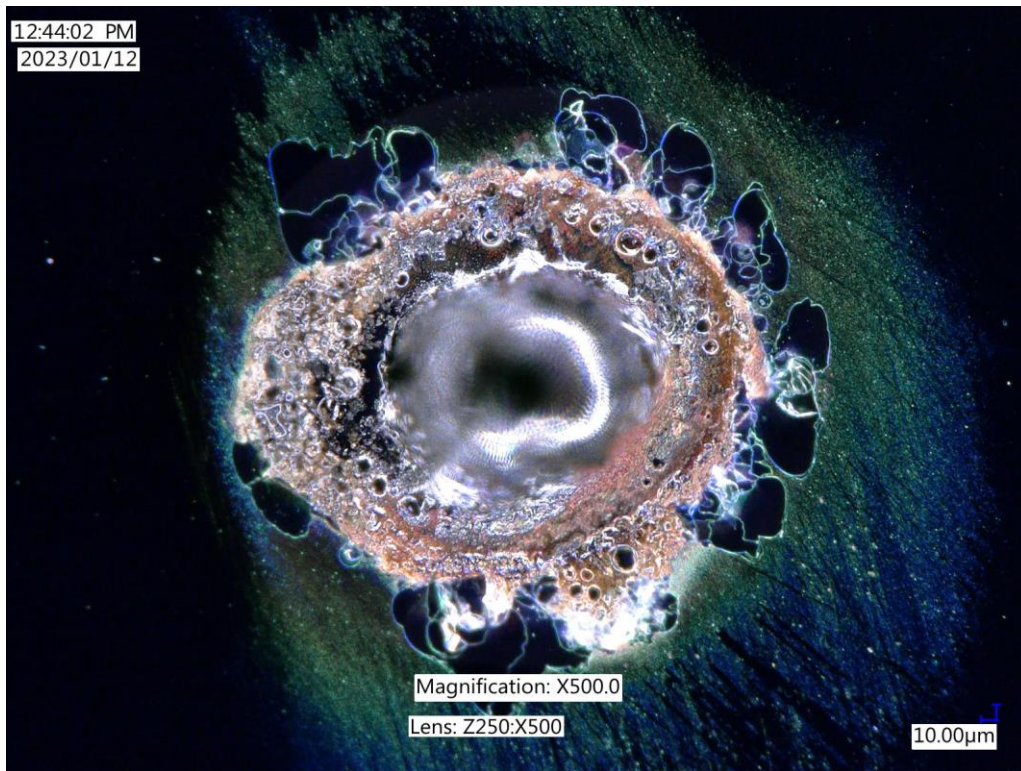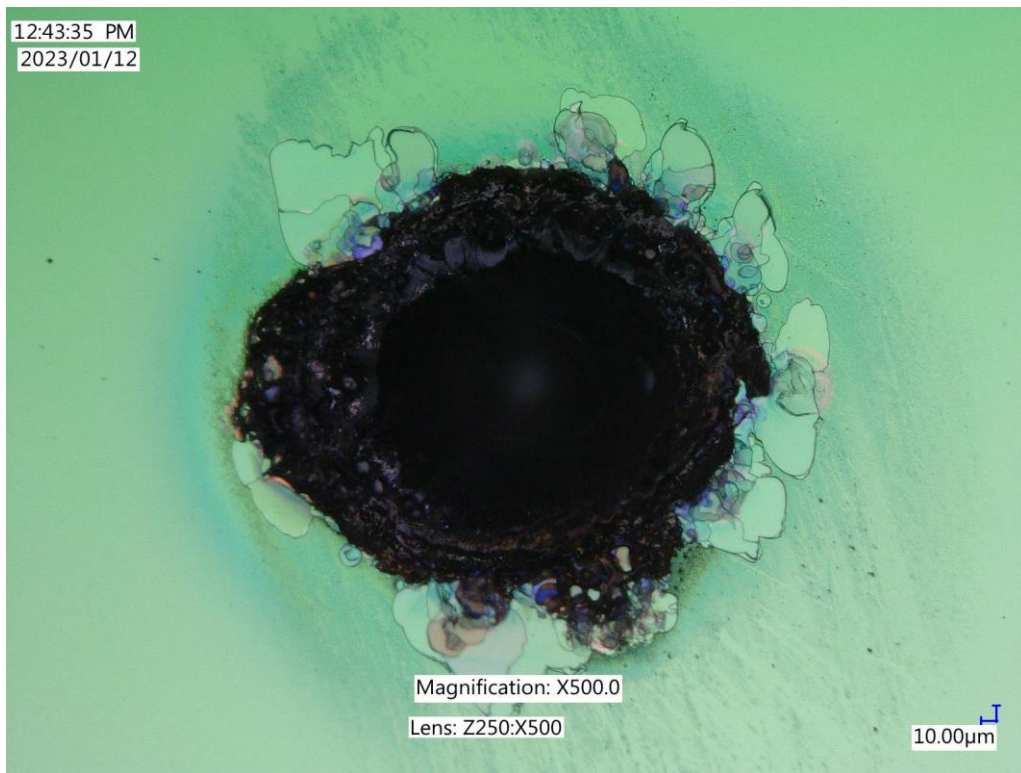

ITM09 point-f

12:49:36 PM
2023/01/12



Magnification: X500.0

Lens: Z250:X500

10.00µm

12:50:02 PM
2023/01/12



Magnification: X500.0

Lens: Z250:X500

10.00µm

ITM09 point-g

12:53:52 PM
2023/01/12



Magnification: X1000.0
Lens: Z250:X1000

10.00µm

12:54:22 PM
2023/01/12





Magnification: X1000.0
Lens: Z250:X1000

10.00µm

ITM09 point-h



ITM09 point-i

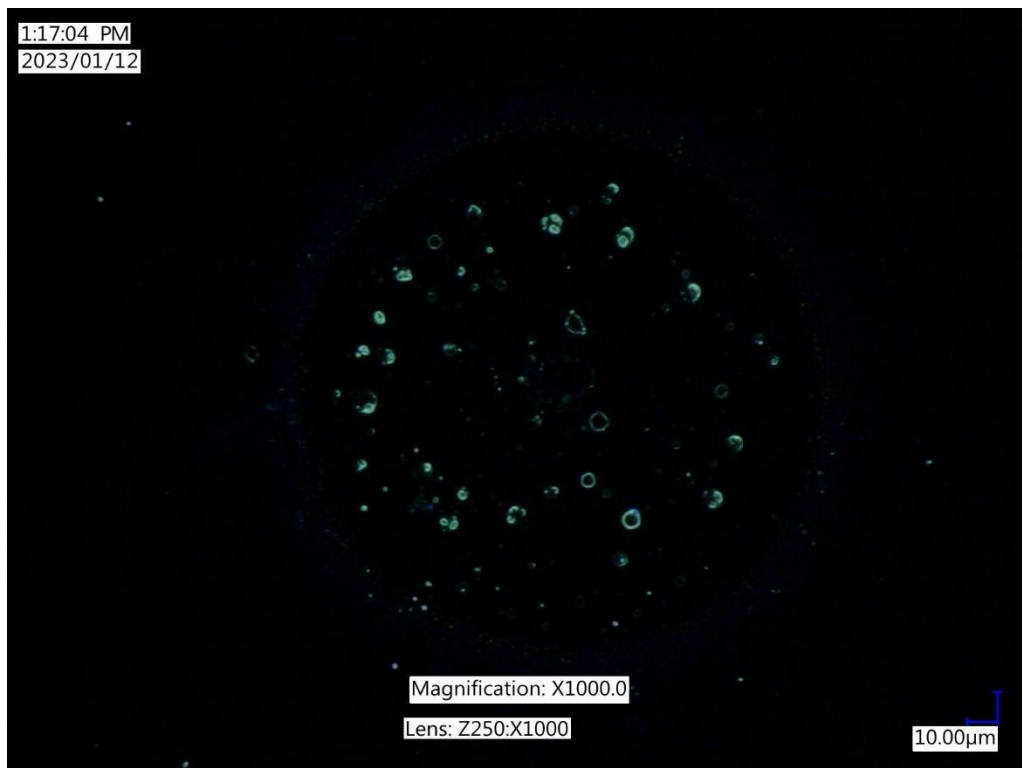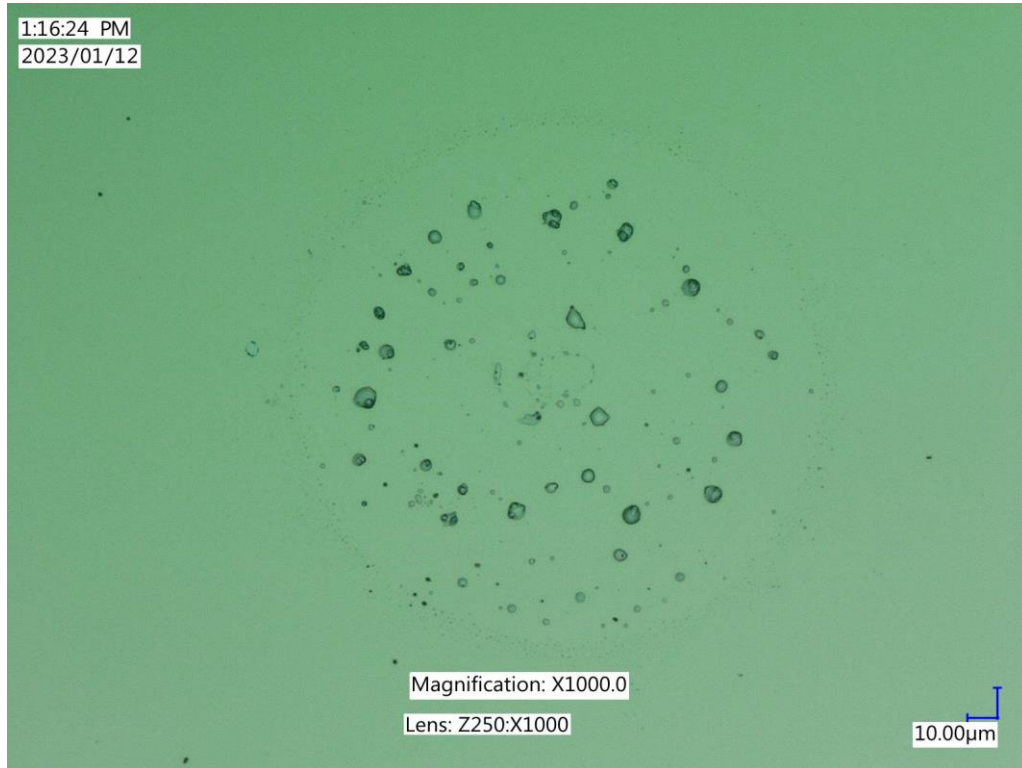

ITM09 point-j



ITM09 point-k



ITM09 point-l

