



ETM14 HR TIS measurement ( $\phi_{\text{beam}} = 0.3 \text{ mm}$ , Step= 1.0 mm)

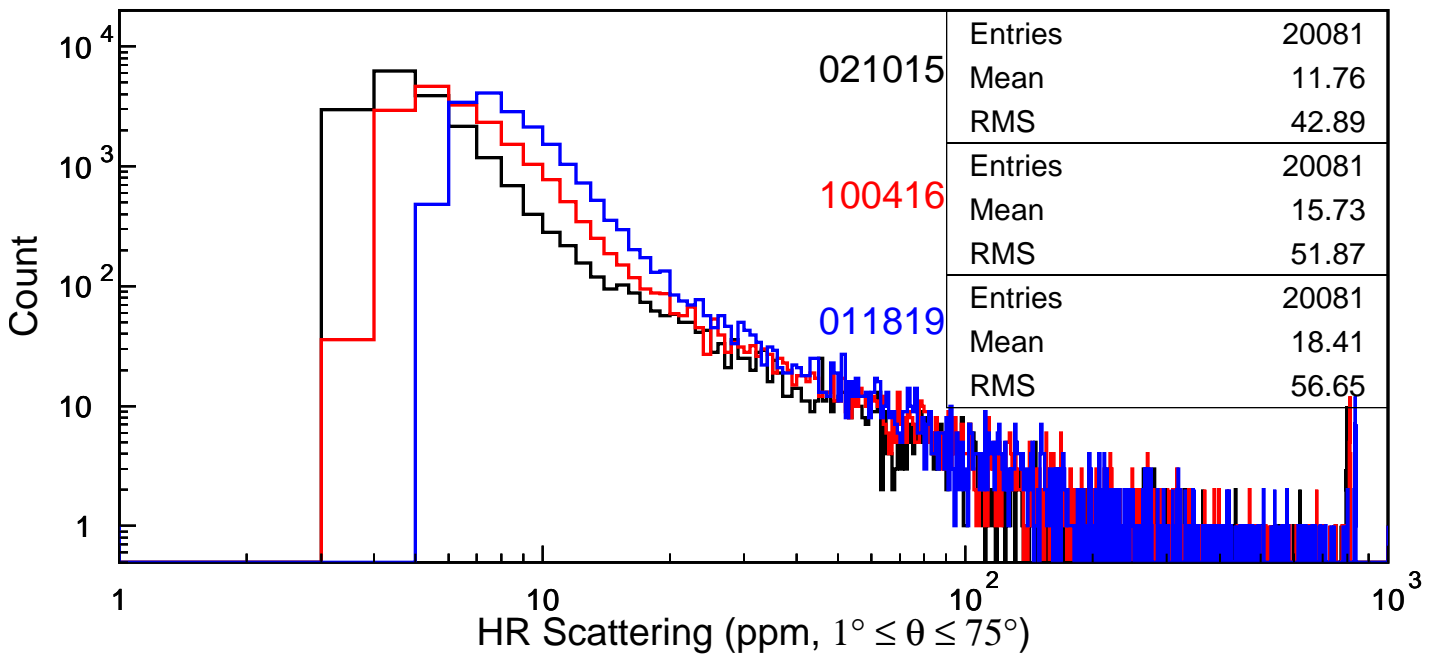

ETM14 HR TIS measurement ( $\phi_{\text{beam}} = 0.3 \text{ mm}$ , Step= 0.3 mm)

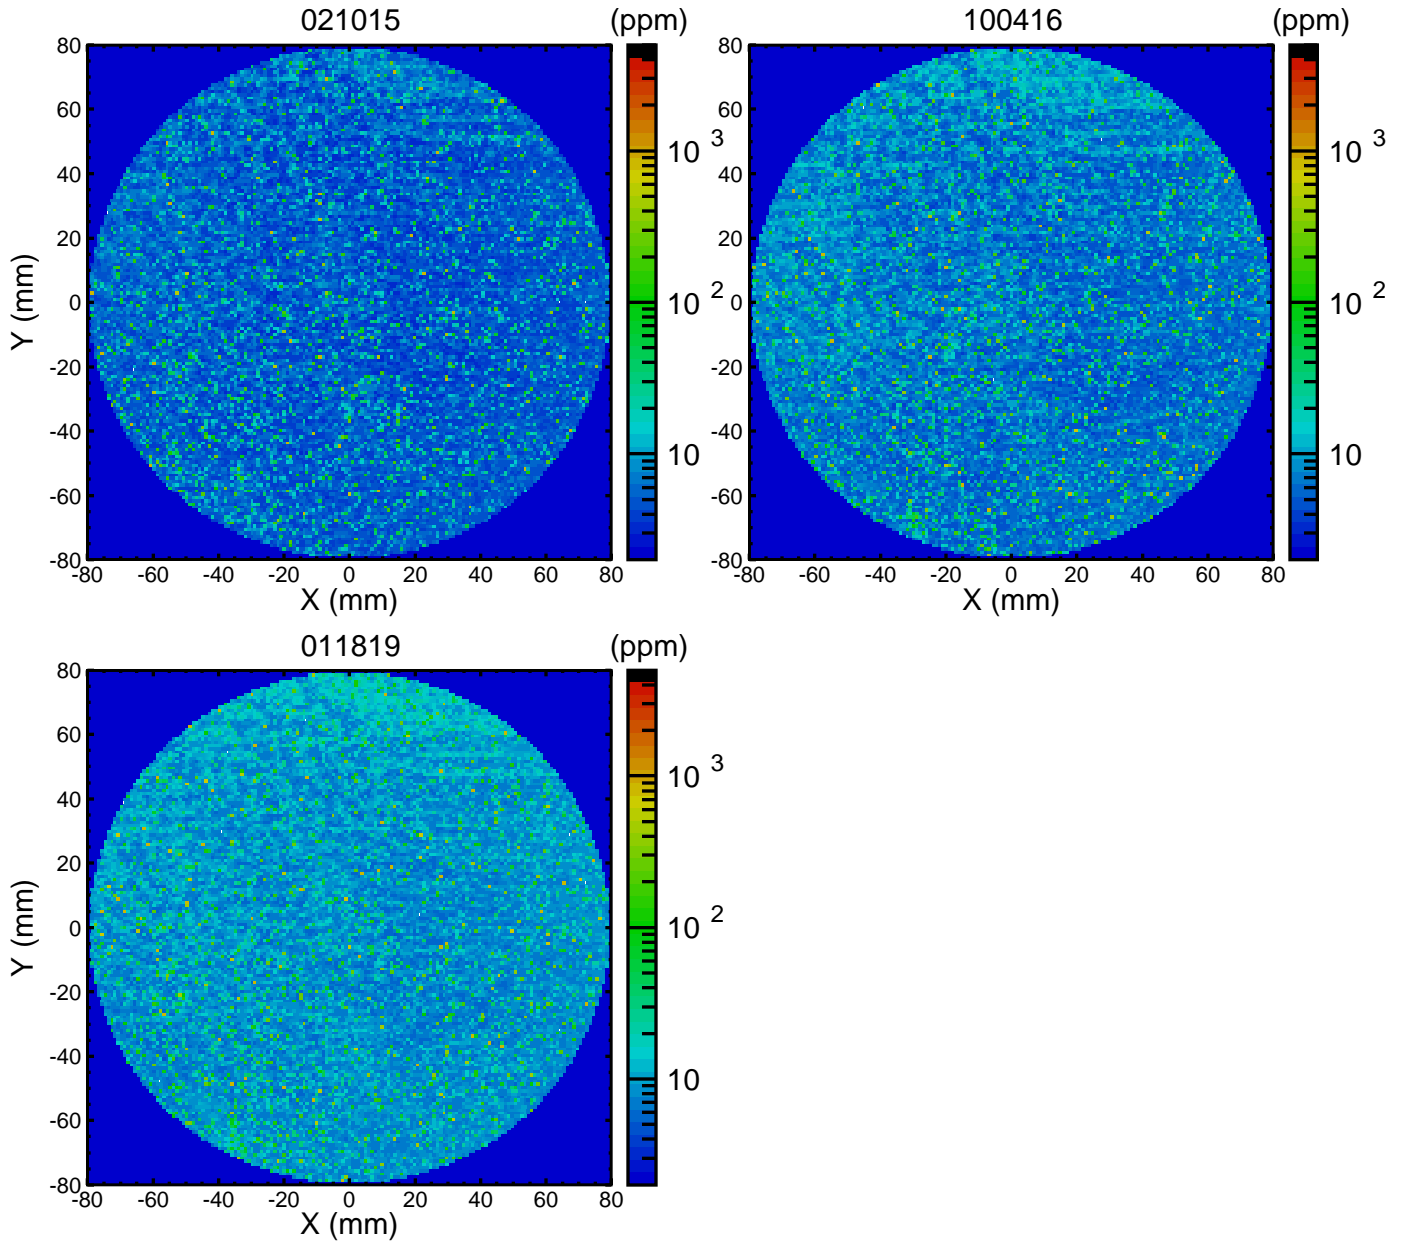